

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015244.D
 Acq On : 23 May 2023 17:06
 Operator : CG/JU
 Sample : 02861-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FM2

Quant Time: May 23 17:47:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 23 01:25:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	193204	20.000	ng/ul	0.00
20) Naphthalene-d8	10.952	136	845161	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	532231	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1068634	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	737944	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	781062	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.429	96	29329	5.898	ng/uL	0.00
4) Pyridine-d5	3.876	84	79424	5.635	ng/ul	0.00
7) Phenol-d5	7.269	99	187968	10.478	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	333104	32.152	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	370328	28.078	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	296402	20.736	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	222868	33.558	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	241524	32.684	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	417721	31.327	ng/ul	0.00
31) 4-Chloroaniline-d4	11.087	131	219019	11.101	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	1516892	37.716	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1666349	36.227	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	59177	7.578	ng/ul	0.00
60) Fluorene-d10	15.751	176	1261137	37.161	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	176050	26.141	ng/ul	0.00
73) Anthracene-d10	17.610	188	1886248	38.547	ng/ul	0.00
81) Pyrene-d10	19.828	212	1931239	45.123	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1607537	41.461	ng/ul	0.00
Target Compounds						
39) 1,2,4,5-Tetrachloroben...	12.963	216	17528	1.101	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015244.D
Acq On : 23 May 2023 17:06
Operator : CG/JU
Sample : 02861-21
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FM2

Quant Time: May 23 17:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

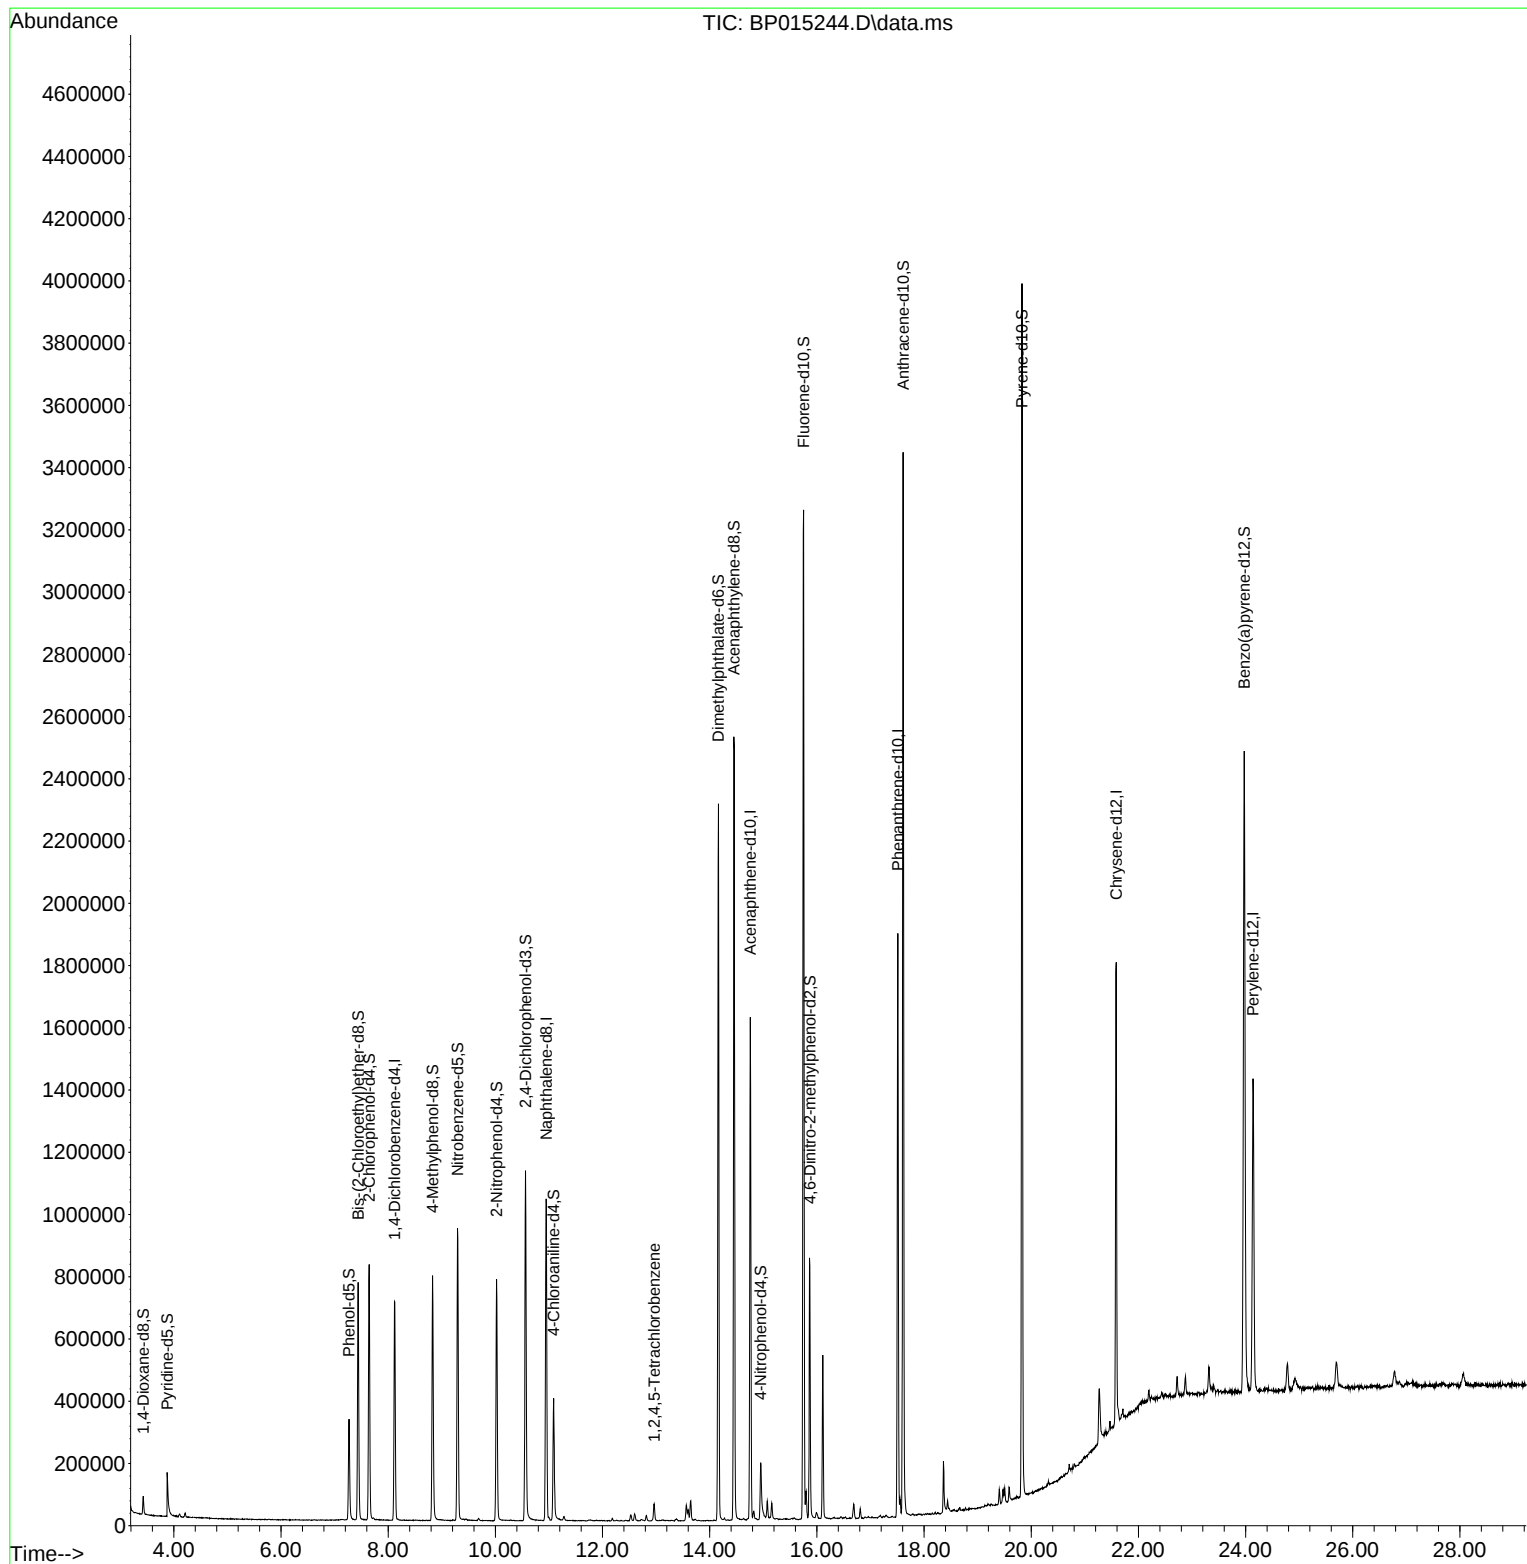

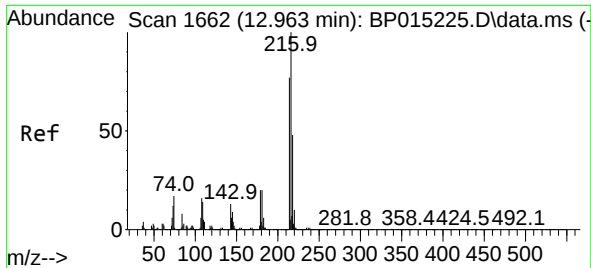

#39

1,2,4,5-Tetrachlorobenzene

Concen: 1.101 ng/ul

RT: 12.963 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP015244.D


Acq: 23 May 2023 17:06

Instrument :

BNA_P

ClientSampleId :

H0FM2

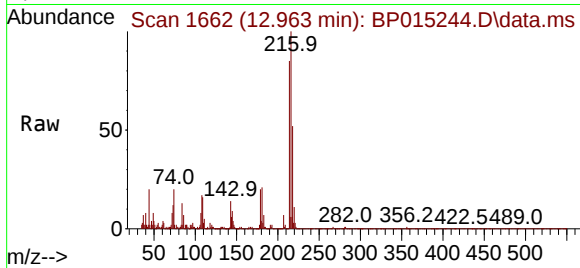

Tgt Ion:216 Resp: 17528

Ion Ratio Lower Upper

216 100

214 84.6 61.4 92.0

179 20.4 15.9 23.9

108 16.9 13.7 20.5

