




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015238.D
Acq On : 23 May 2023 13:44
Operator : CG/JU
Sample : 02861-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FLO

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 23 15:31:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

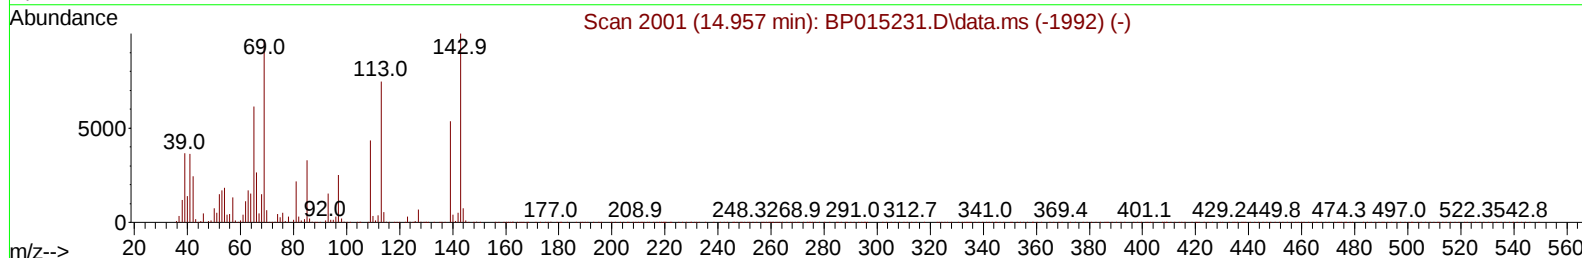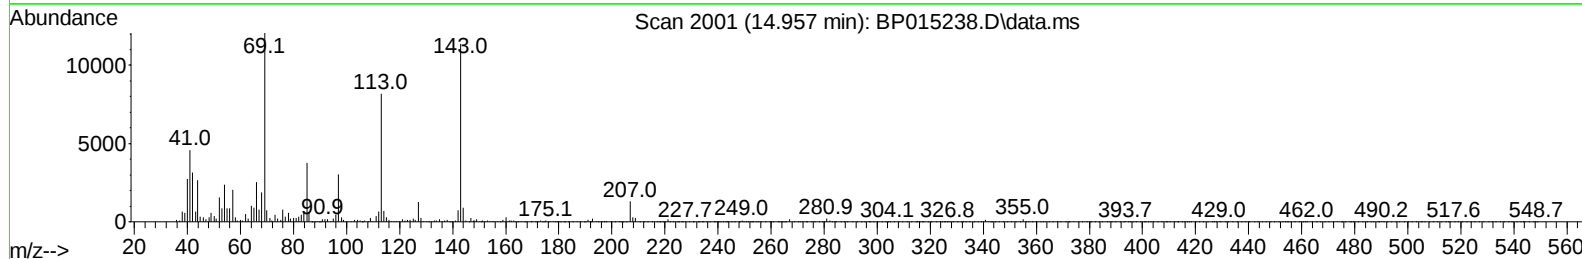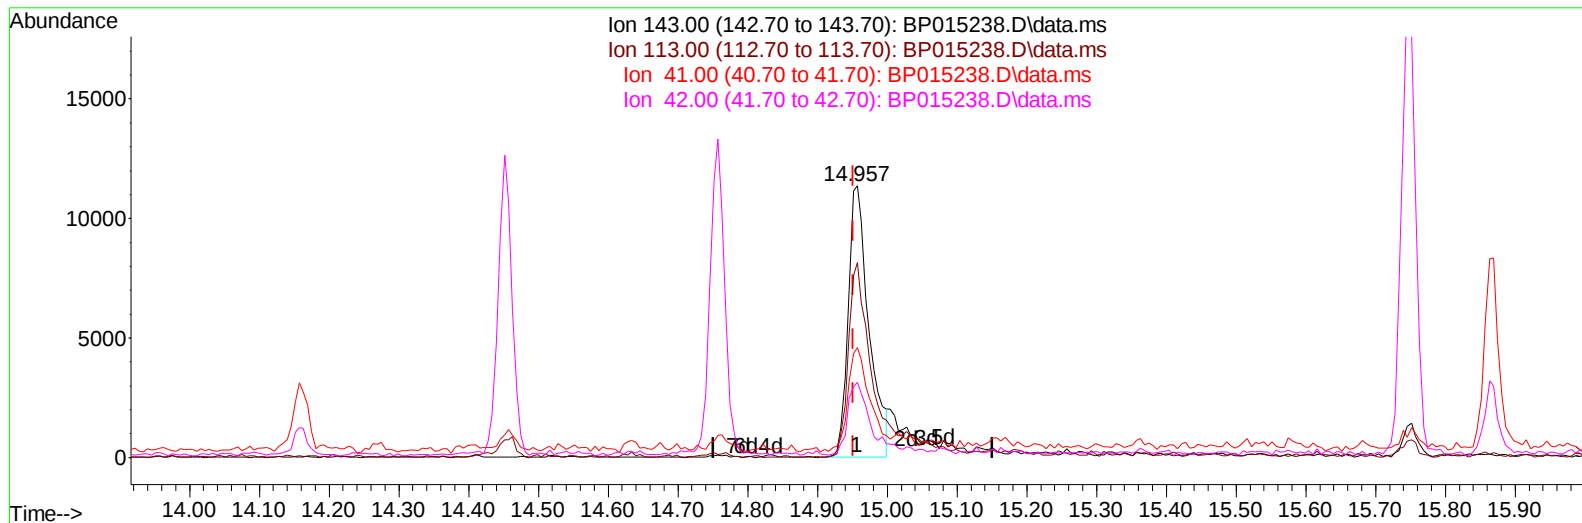

TIC: BP015238.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.957min (+ 0.006) 2.54 ng/u1

response 23407

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.30	71.88
41.00	36.10	40.45
42.00	24.50	27.80




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015238.D
 Acq On : 23 May 2023 13:44
 Operator : CG/JU
 Sample : 02861-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FLO

Manual IntegrationsAPPROVED

Quant Time: May 23 15:31:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 23 01:25:41 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/24/2023
 Supervised By :mohammad ahmed 05/24/2023

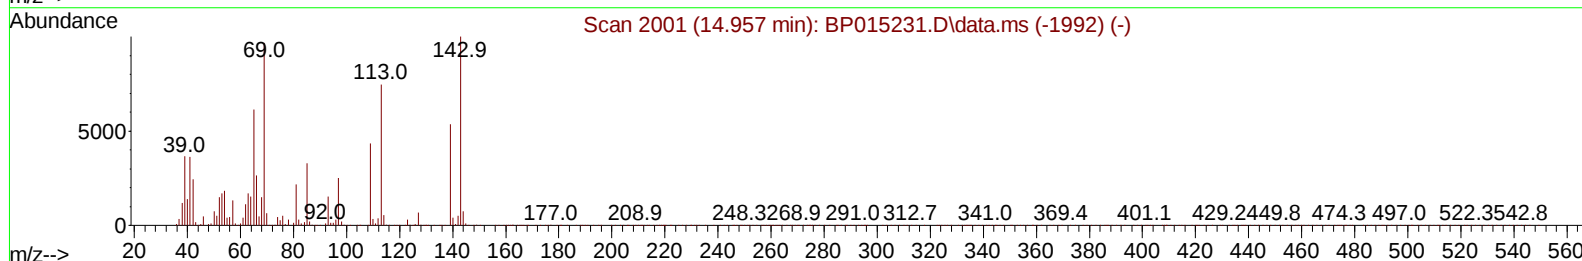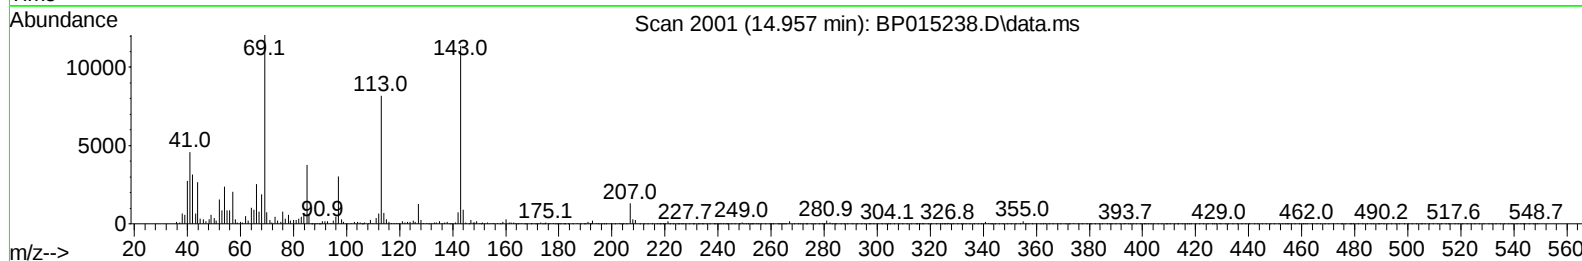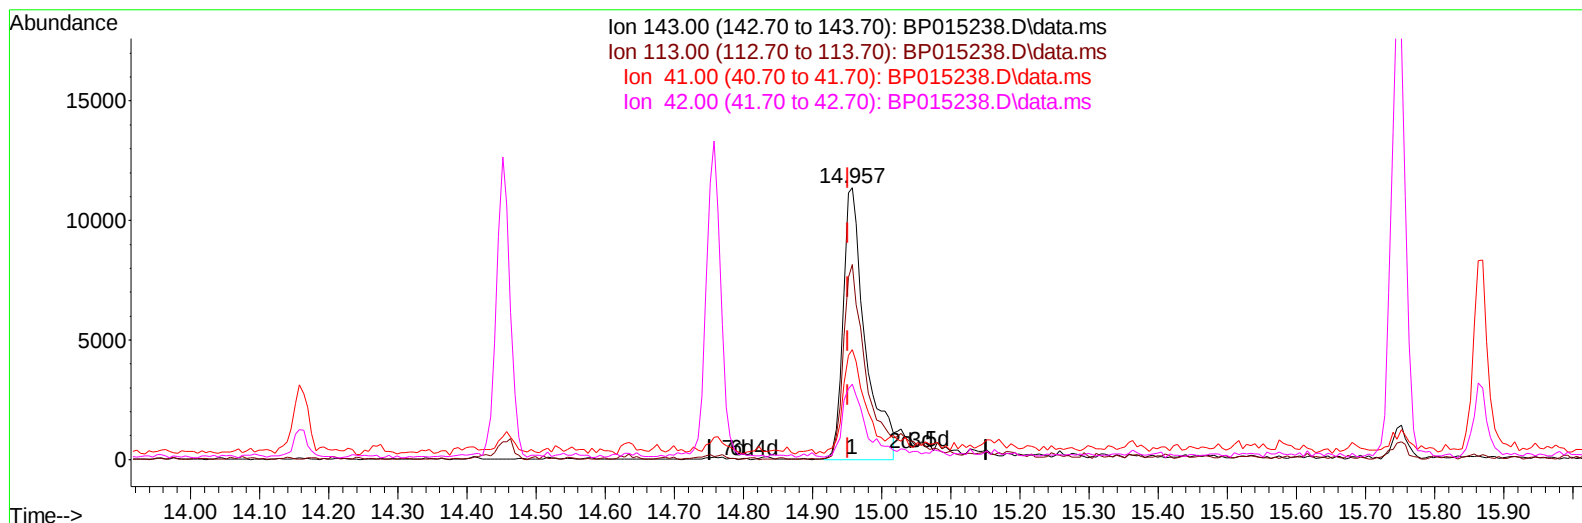

TIC: BP015238.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.957min (+ 0.006) 2.74 ng/ul m

response 25226

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.30	71.88
41.00	36.10	40.45
42.00	24.50	27.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015238.D
 Acq On : 23 May 2023 13:44
 Operator : CG/JU
 Sample : 02861-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOFLO

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
 Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 23 23:00:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 23 01:25:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	224721	20.000	ng/ul	0.00
20) Naphthalene-d8	10.951	136	987883	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	627963	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1283576	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	897191	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	975876	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	23381	4.042	ng/uL	0.00
4) Pyridine-d5	3.875	84	126883	7.739	ng/ul	0.00
7) Phenol-d5	7.269	99	104752	5.021	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	313198	25.990	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	303542	19.786	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	202700	12.192	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	206322	26.579	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	218554	25.303	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	367017	23.548	ng/ul	0.00
31) 4-Chloroaniline-d4	11.087	131	464337	20.135	ng/ul	0.00
46) Dimethylphthalate-d6	14.163	166	1361649	28.695	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1450953	26.735	ng/ul	0.00
54) 4-Nitrophenol-d4	14.957	143	25226m	2.738	ng/ul	0.00
60) Fluorene-d10	15.745	176	1110442	27.733	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	144551	17.870	ng/ul	0.00
73) Anthracene-d10	17.610	188	1704039	28.992	ng/ul	0.00
81) Pyrene-d10	19.827	212	1803451	34.658	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	1509180	31.153	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015238.D
Acq On : 23 May 2023 13:44
Operator : CG/JU
Sample : 02861-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FLO

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 23 23:00:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

