




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015261.D
Acq On : 24 May 2023 03:08
Operator : CG/JU
Sample : 02861-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FL9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 24 04:11:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

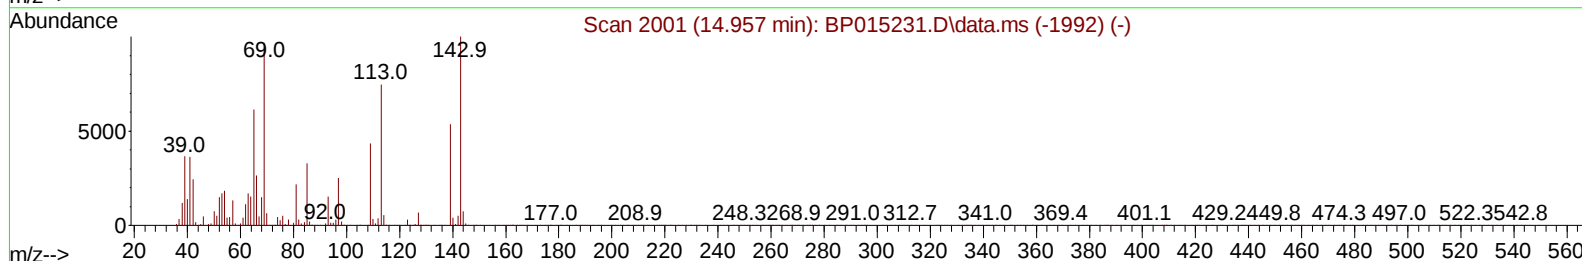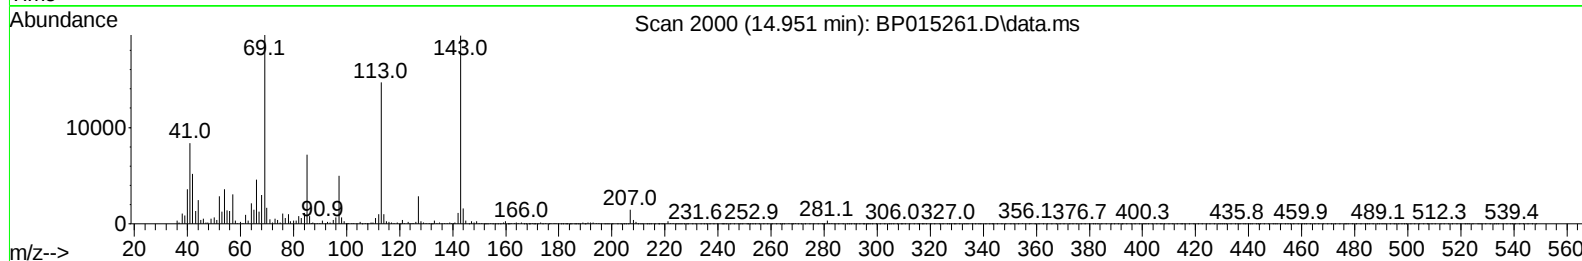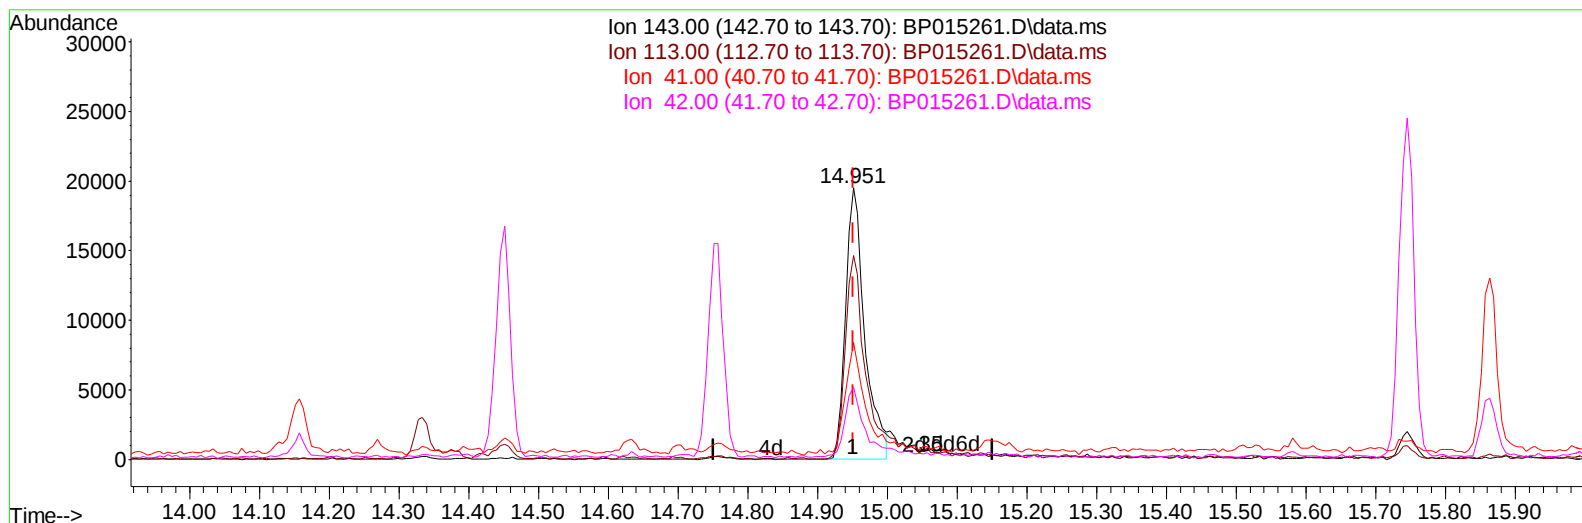

TIC: BP015261.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.951min (-0.000) 3.43 ng/u1****response 37176**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.30	75.12
41.00	36.10	43.00
42.00	24.50	26.50




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015261.D
Acq On : 24 May 2023 03:08
Operator : CG/JU
Sample : 02861-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FL9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 24 04:11:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

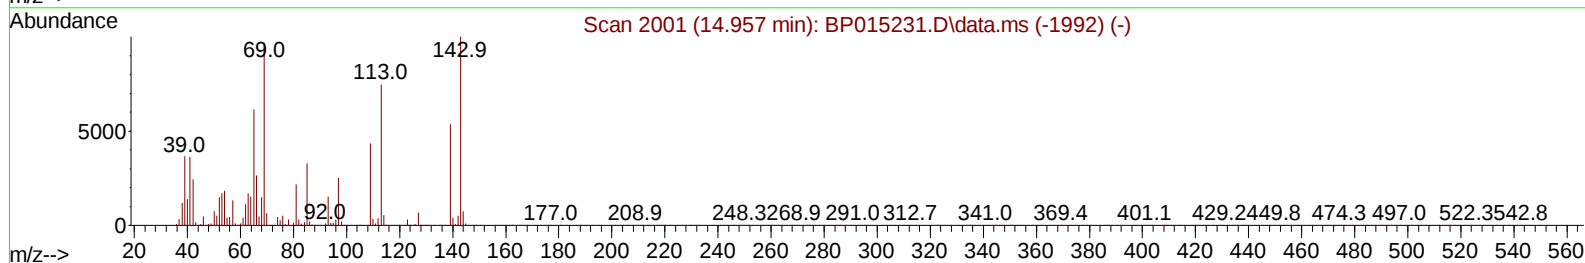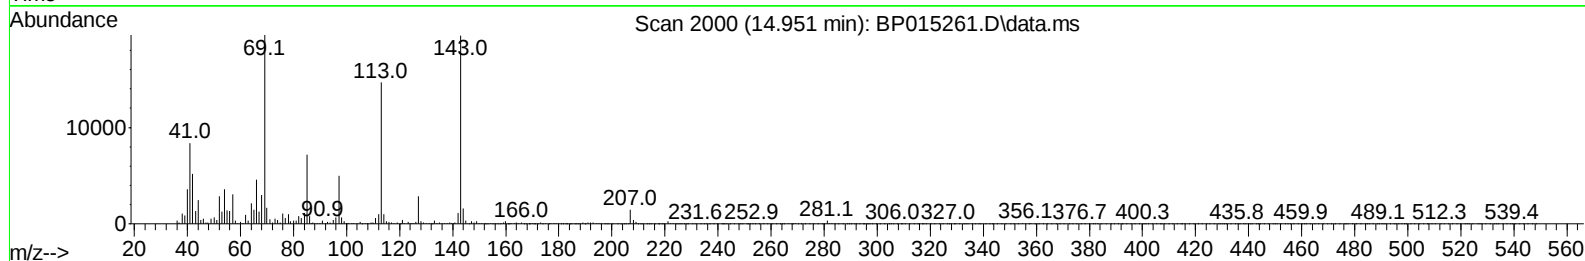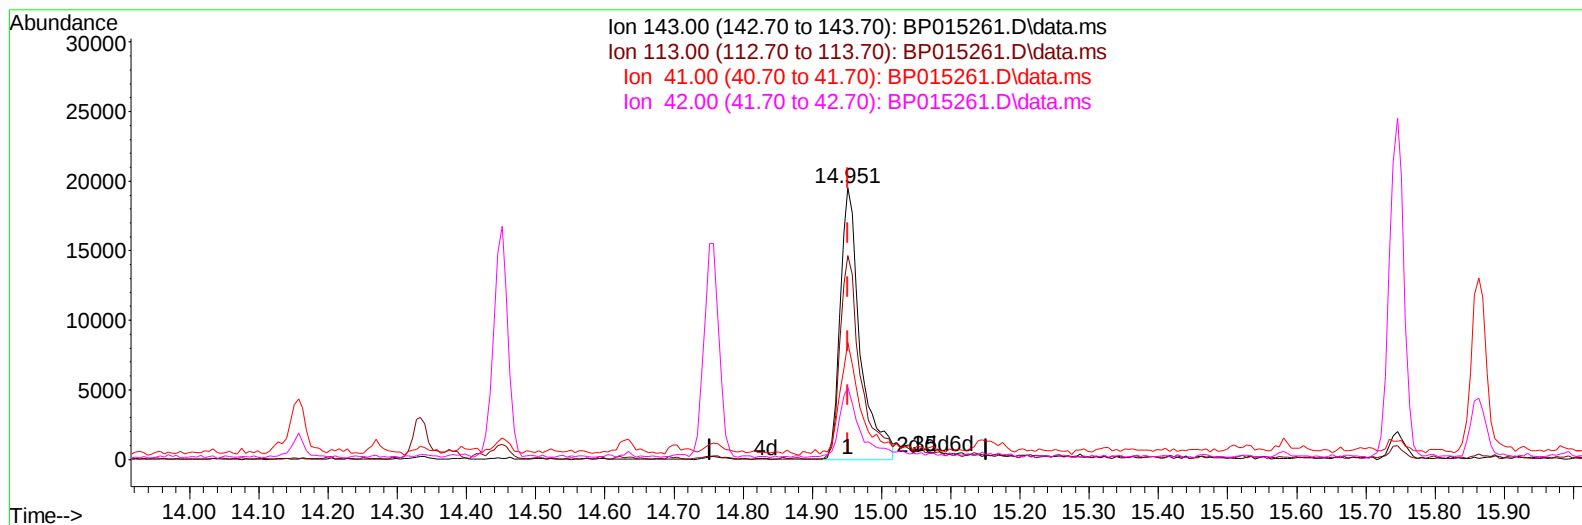

TIC: BP015261.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.951min (-0.000) 3.60 ng/u1 m

response 39027

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.30	75.12
41.00	36.10	43.00
42.00	24.50	26.50

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015261.D
 Acq On : 24 May 2023 03:08
 Operator : CG/JU
 Sample : 02861-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FL9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
 Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 24 04:17:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 23 01:25:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.116	152	263800	20.000	ng/ul	0.00
20) Naphthalene-d8	10.946	136	1171504	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	739271	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1610465	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1183590	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	1205069	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	24172	3.560	ng/uL	0.00
4) Pyridine-d5	3.869	84	139071	7.226	ng/ul	0.00
7) Phenol-d5	7.263	99	122070	4.984	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.434	67	382694	27.053	ng/ul	0.00
11) 2-Chlorophenol-d4	7.640	132	368388	20.456	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	244828	12.544	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	258889	28.123	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	275212	26.868	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.557	165	465926	25.208	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	415806	15.205	ng/ul	0.00
46) Dimethylphthalate-d6	14.157	166	1815971	32.507	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1931528	30.231	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	39027m	3.598	ng/ul	0.00
60) Fluorene-d10	15.745	176	1482641	31.453	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	227559	22.421	ng/ul	0.00
73) Anthracene-d10	17.610	188	2381065	32.288	ng/ul	0.00
81) Pyrene-d10	19.827	212	2675007	38.968	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	2103072	35.156	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015261.D
Acq On : 24 May 2023 03:08
Operator : CG/JU
Sample : 02861-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FL9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/24/2023
Supervised By :mohammad ahmed 05/24/2023

Quant Time: May 24 04:17:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

