

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015235.D
 Acq On : 23 May 2023 12:03
 Operator : CG/JU
 Sample : 02861-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FK7

Quant Time: May 23 13:37:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 23 01:25:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	229129	20.000	ng/u1	0.00
20) Naphthalene-d8	10.952	136	1007533	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	650932	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	1380598	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	971464	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	999419	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	24775	4.201	ng/uL	0.00
4) Pyridine-d5	3.875	84	127048	7.600	ng/u1	0.00
7) Phenol-d5	7.269	99	95301	4.480	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	316854	25.788	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	292872	18.724	ng/u1	0.00
15) 4-Methylphenol-d8	8.828	113	196594	11.597	ng/u1	0.00
21) Nitrobenzene-d5	9.299	128	208431	26.327	ng/u1	0.00
24) 2-Nitrophenol-d4	10.022	143	217784	24.722	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	373529	23.498	ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	475629	20.223	ng/u1	0.00
46) Dimethylphthalate-d6	14.163	166	1421471	28.899	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	1525863	27.123	ng/u1	0.00
54) 4-Nitrophenol-d4	14.951	143	27010	2.828	ng/u1	0.00
60) Fluorene-d10	15.751	176	1171847	28.234	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.869	200	71816	8.254	ng/u1	0.00
73) Anthracene-d10	17.610	188	1931157	30.547	ng/u1	0.00
81) Pyrene-d10	19.828	212	2118635	37.602	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	1698385	34.233	ng/u1	0.00
Target Compounds						
					Qvalue	
18) 4-Methylphenol	8.887	108	34425	1.855	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015235.D
Acq On : 23 May 2023 12:03
Operator : CG/JU
Sample : 02861-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FK7

Quant Time: May 23 13:37:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 23 01:25:41 2023
Response via : Initial Calibration

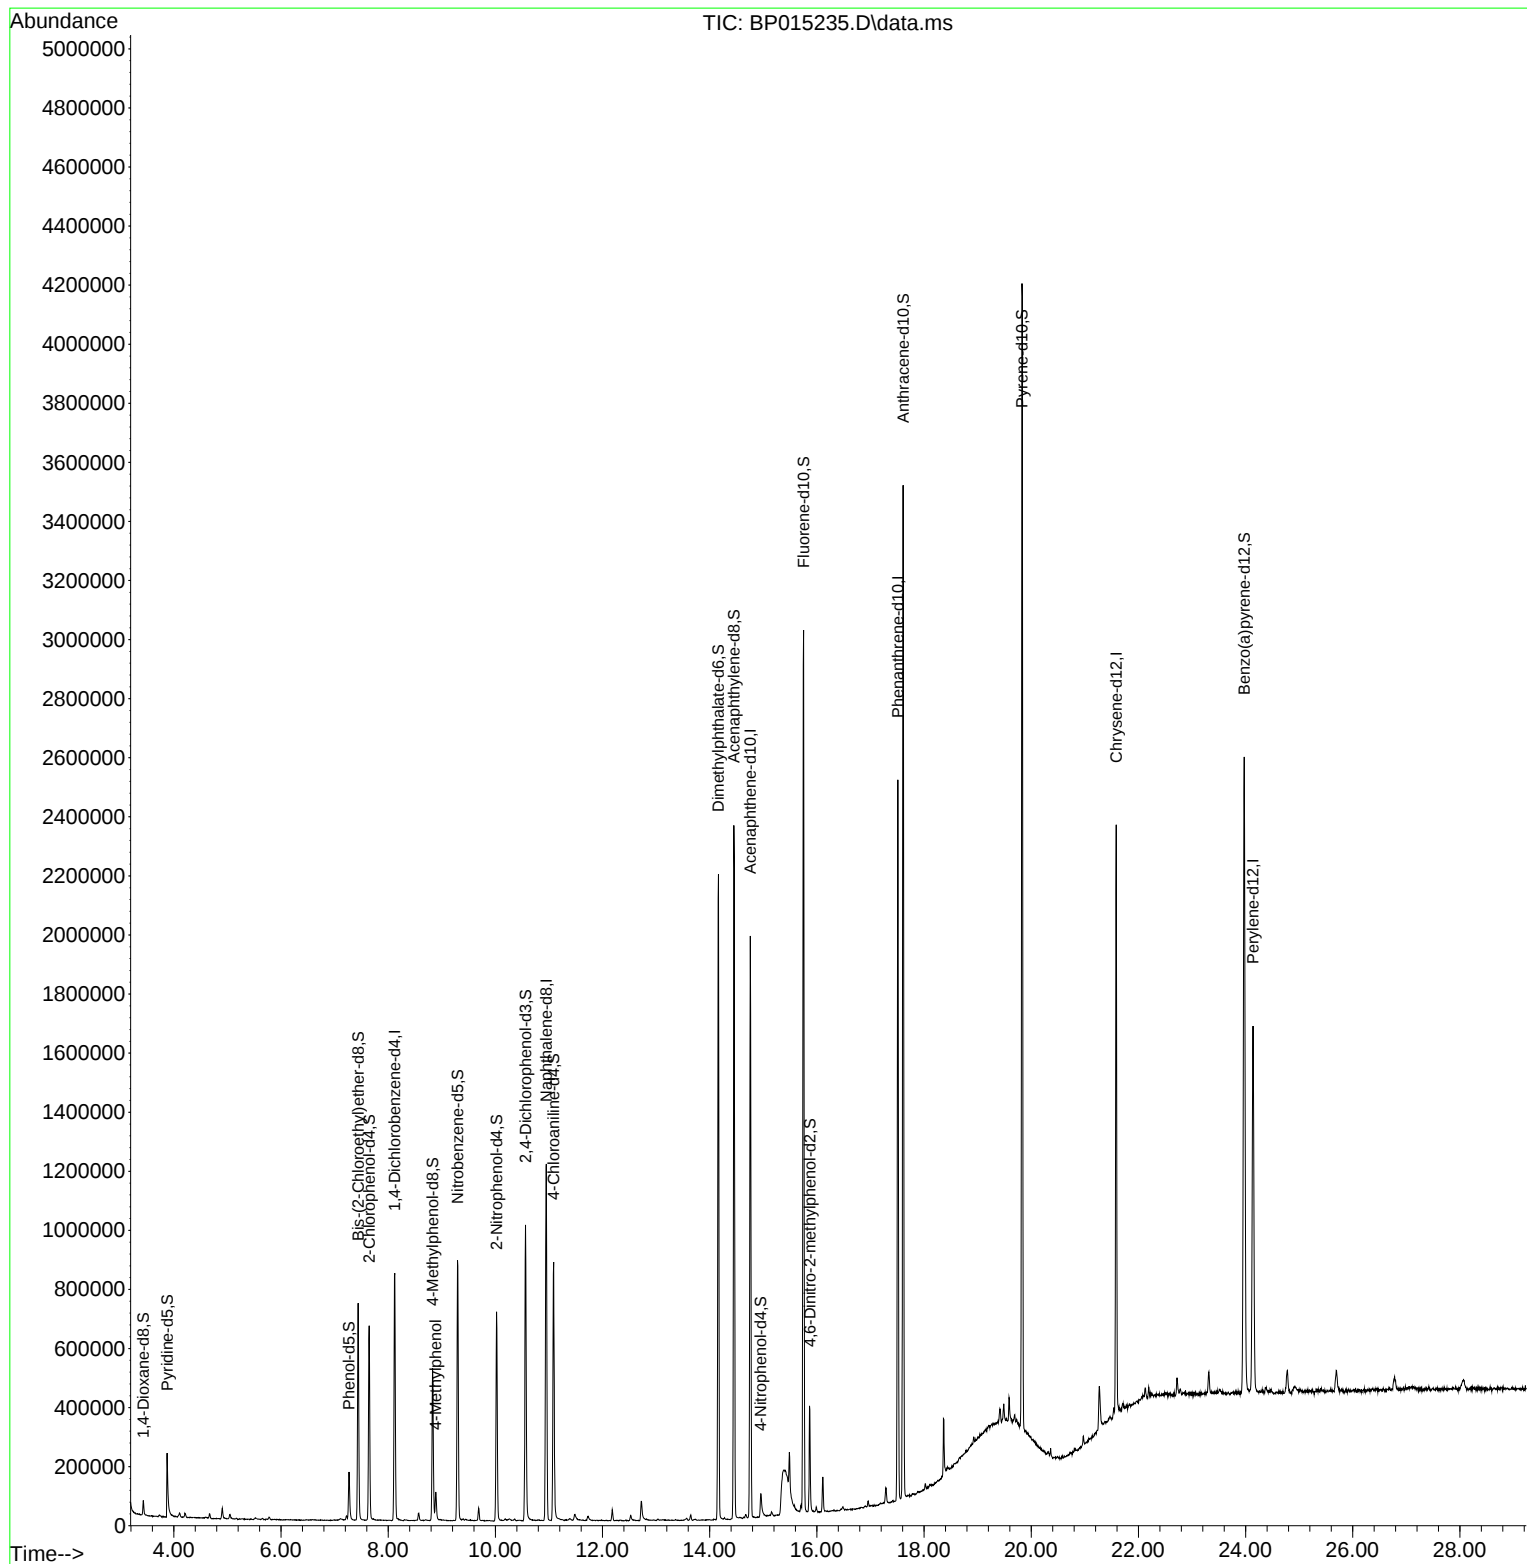

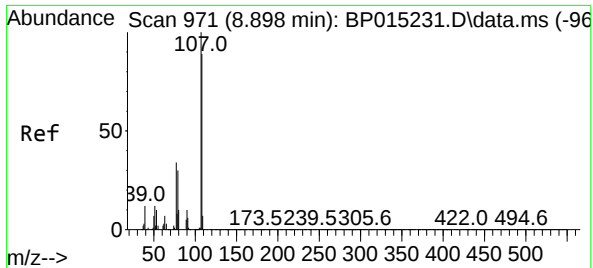

#18
4-Methylphenol
Concen: 1.855 ng/ul
RT: 8.887 min Scan# 90
Delta R.T. -0.012 min
Lab File: BP015235.D
Acq: 23 May 2023 12:03

Instrument :
BNA_P
ClientSampleId :
H0FK7

Tgt Ion:108 Resp: 34425
Ion Ratio Lower Upper
108 100
107 120.5 88.5 132.7

