

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015232.D
 Acq On : 23 May 2023 10:22
 Operator : CG/JU
 Sample : PB152971BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK971

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	51	rVB	72182	101190	2.04%	0.170%
2	3.863	112	115	135	rBV	813342	1327468	26.74%	2.231%
3	4.211	171	174	180	rVB	11614	16501	0.33%	0.028%
4	4.705	254	258	259	rBV4	4084	5662	0.11%	0.010%
5	7.269	687	694	708	rBV	1051103	1700078	34.25%	2.857%
6	7.440	716	723	735	rBV	881230	1355553	27.31%	2.278%
7	7.646	751	758	773	rBV	1078243	1723168	34.71%	2.896%
8	8.122	831	839	851	rVB	778510	1280497	25.79%	2.152%
9	8.828	953	959	973	rVV	1298551	2208765	44.49%	3.712%
10	9.298	1029	1039	1050	rBV	1040011	1757308	35.40%	2.953%
11	10.022	1154	1162	1173	rBV	917107	1539680	31.01%	2.587%
12	10.563	1246	1254	1273	rBV	1351854	2339070	47.12%	3.931%
13	10.945	1312	1319	1330	rBV	1171834	1973280	39.75%	3.316%
14	11.087	1335	1343	1360	rBV	1293307	2305969	46.45%	3.875%
15	12.534	1583	1589	1599	rBV2	18524	40177	0.81%	0.068%
16	13.645	1773	1778	1784	rVB2	22578	34588	0.70%	0.058%
17	13.739	1789	1794	1800	rVB5	4571	7685	0.15%	0.013%
18	14.163	1859	1866	1880	rBV	2443760	3370587	67.90%	5.664%
19	14.451	1908	1915	1929	rBV	2645865	4089416	82.37%	6.872%
20	14.757	1960	1967	1976	rBV	1787285	2658477	53.55%	4.467%
21	14.951	1990	2000	2025	rBV	716211	1380344	27.80%	2.319%
22	15.163	2034	2036	2044	rVB8	7146	12168	0.25%	0.020%
23	15.751	2129	2136	2149	rBV	3325262	4888064	98.46%	8.214%
24	15.869	2149	2156	2165	rBV	819492	1132758	22.82%	1.903%
25	15.986	2171	2176	2182	rVB4	18166	31669	0.64%	0.053%
26	16.316	2228	2232	2238	rBV9	3473	6703	0.14%	0.011%
27	16.533	2267	2269	2274	rVB6	5061	6075	0.12%	0.010%
28	17.186	2374	2380	2383	rBV8	6828	11779	0.24%	0.020%
29	17.304	2396	2400	2405	rBV5	4144	7636	0.15%	0.013%
30	17.510	2428	2435	2446	rBV	2084706	2995429	60.34%	5.033%
31	17.610	2446	2452	2464	rVV	3498082	4925040	99.21%	8.276%
32	19.404	2753	2757	2762	rBV3	43615	69533	1.40%	0.117%
33	19.474	2766	2769	2775	rVB	36910	52410	1.06%	0.088%
34	19.827	2824	2829	2837	rBV	3730938	4964400	100.00%	8.342%
35	21.586	3123	3128	3138	rBV	1704899	2398412	48.31%	4.030%
36	23.974	3527	3534	3546	rVB2	2029791	4375435	88.14%	7.352%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015232.D
Acq On : 23 May 2023 10:22
Operator : CG/JU
Sample : PB152971BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK971

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	24.139	3556	3562	3575	rVB	1118477	2417563	48.70%	4.062%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 59510537

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015232.D
Acq On : 23 May 2023 10:22
Operator : CG/JU
Sample : PB152971BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK971

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

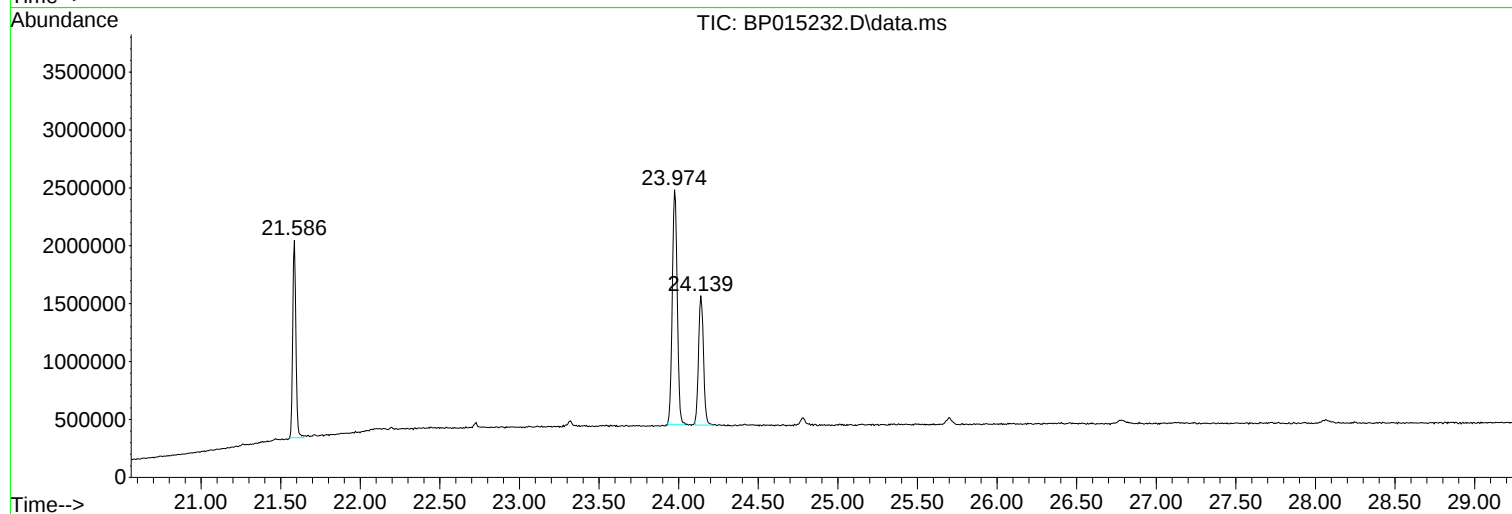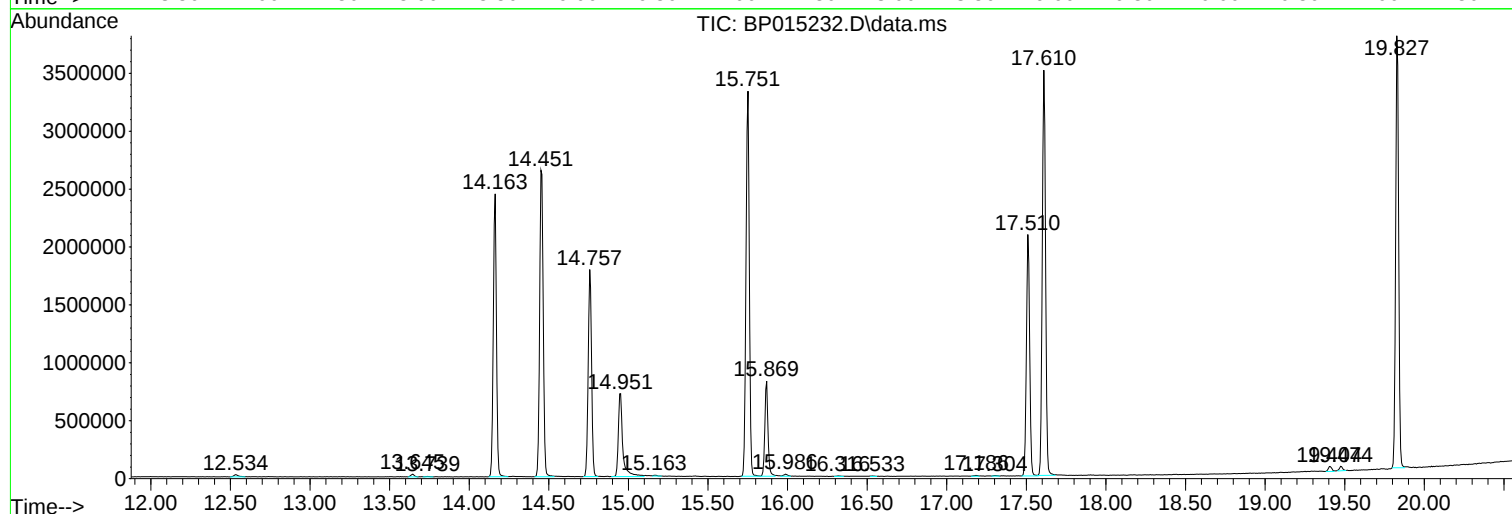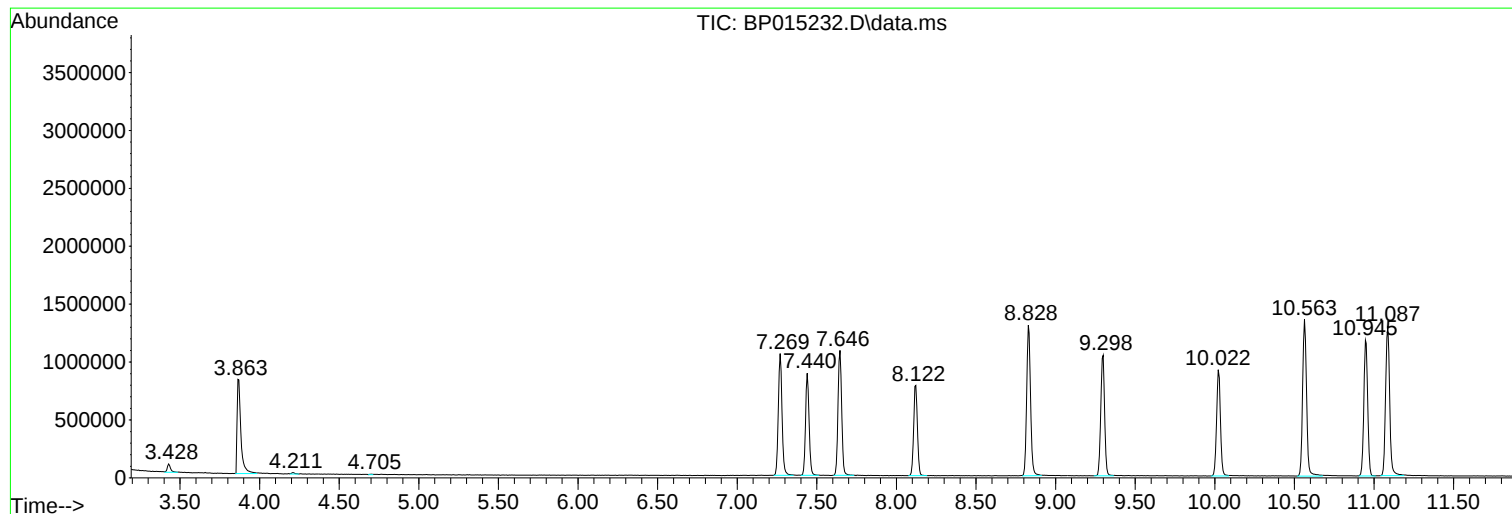

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015232.D
Acq On : 23 May 2023 10:22
Operator : CG/JU
Sample : PB152971BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK971

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015232.D
Acq On : 23 May 2023 10:22
Operator : CG/JU
Sample : PB152971BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK971

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------