

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015233.D
 Acq On : 23 May 2023 10:56
 Operator : CG/JU
 Sample : PB152973BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK973

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	48	rVB	67390	87319	1.64%	0.142%
2	3.864	113	115	136	rBV	813598	1311096	24.56%	2.139%
3	4.211	170	174	180	rVB2	11854	19706	0.37%	0.032%
4	7.269	687	694	713	rBV	1019325	1645602	30.83%	2.685%
5	7.440	716	723	734	rVB	836139	1299492	24.34%	2.120%
6	7.646	750	758	768	rBV	1027144	1659839	31.09%	2.708%
7	8.122	828	839	850	rBV	795784	1303556	24.42%	2.127%
8	8.828	949	959	976	rBV	1337369	2270614	42.54%	3.705%
9	9.299	1031	1039	1050	rBV	1045535	1789506	33.52%	2.920%
10	10.022	1153	1162	1177	rBV	934805	1570438	29.42%	2.562%
11	10.563	1246	1254	1276	rBV	1394539	2412823	45.20%	3.937%
12	10.946	1310	1319	1334	rVB	1270355	2138395	40.06%	3.489%
13	11.087	1334	1343	1358	rBV	1311349	2359091	44.19%	3.849%
14	12.534	1583	1589	1599	rBV3	18585	41892	0.78%	0.068%
15	13.640	1773	1777	1783	rBV3	9179	16993	0.32%	0.028%
16	13.740	1789	1794	1798	rVB7	3684	6051	0.11%	0.010%
17	14.163	1858	1866	1876	rBV	2507387	3532227	66.17%	5.763%
18	14.281	1882	1886	1891	rVB8	3723	7051	0.13%	0.012%
19	14.451	1907	1915	1934	rBV	2841287	4309626	80.74%	7.032%
20	14.757	1959	1967	1976	rBV	2037360	2969689	55.63%	4.845%
21	14.945	1991	1999	2020	rBV	721223	1355041	25.38%	2.211%
22	15.163	2034	2036	2045	rVB10	8782	16088	0.30%	0.026%
23	15.751	2129	2136	2150	rBV	3601783	5234258	98.06%	8.540%
24	15.869	2150	2156	2170	rVV	800204	1161594	21.76%	1.895%
25	15.992	2171	2177	2181	rVB3	17011	27872	0.52%	0.045%
26	16.540	2266	2270	2274	rVB7	4151	6133	0.11%	0.010%
27	17.181	2375	2379	2383	rVB7	6142	9797	0.18%	0.016%
28	17.304	2396	2400	2404	rVB5	5115	6571	0.12%	0.011%
29	17.510	2428	2435	2446	rBV	2408266	3399672	63.69%	5.547%
30	17.610	2446	2452	2467	rVV2	3668356	5337983	100.00%	8.709%
31	19.404	2753	2757	2763	rBV	40420	63037	1.18%	0.103%
32	19.475	2766	2769	2776	rVB	35227	55110	1.03%	0.090%
33	19.828	2823	2829	2838	rBV	3593965	4804904	90.01%	7.840%
34	21.586	3123	3128	3144	rBV	1756831	2483525	46.53%	4.052%
35	23.974	3527	3534	3547	rVB2	1938085	4167875	78.08%	6.800%
36	24.145	3556	3563	3572	rVB	1073510	2409261	45.13%	3.931%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015233.D
Acq On : 23 May 2023 10:56
Operator : CG/JU
Sample : PB152973BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK973

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 61289727

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015233.D
Acq On : 23 May 2023 10:56
Operator : CG/JU
Sample : PB152973BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

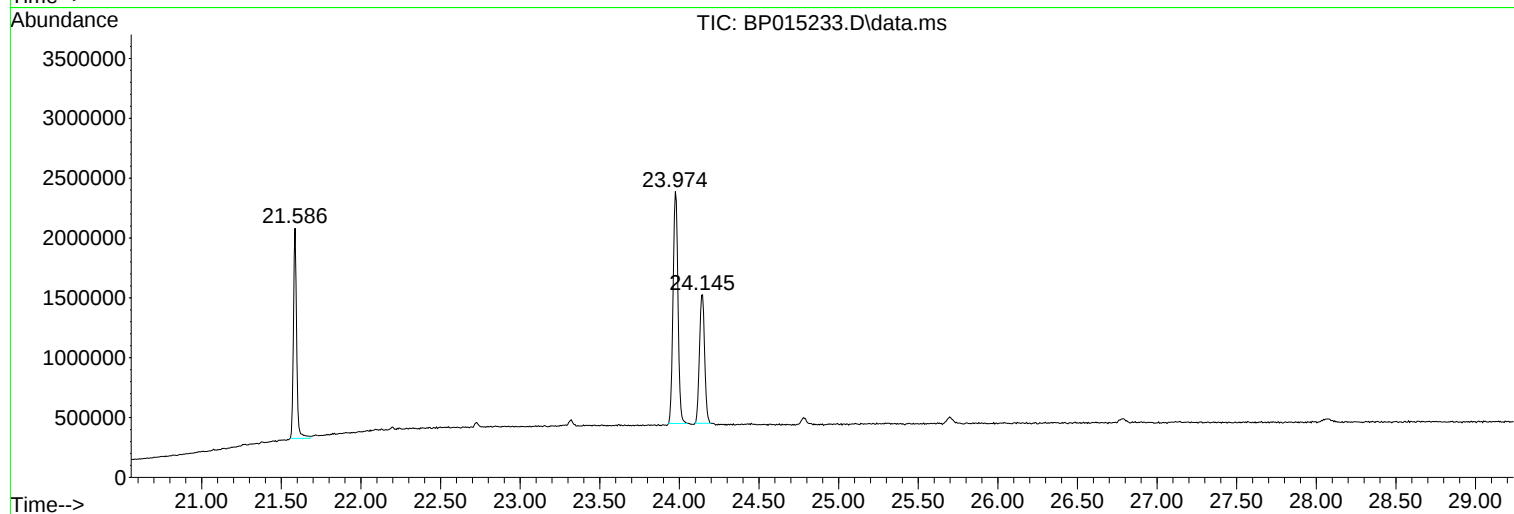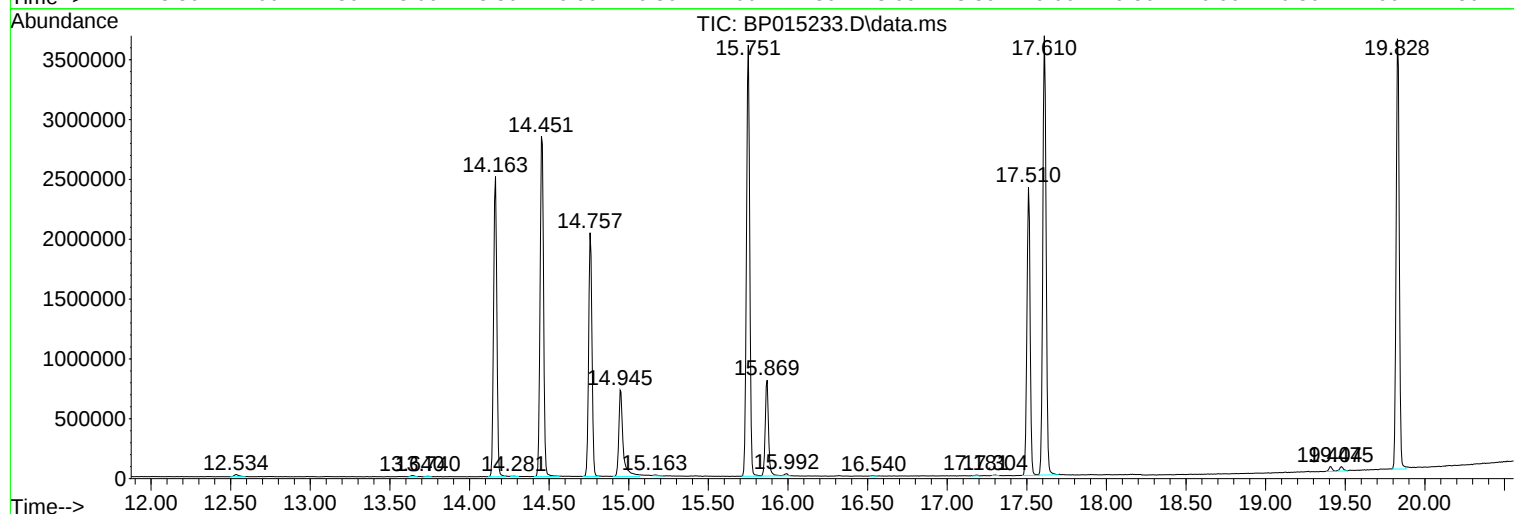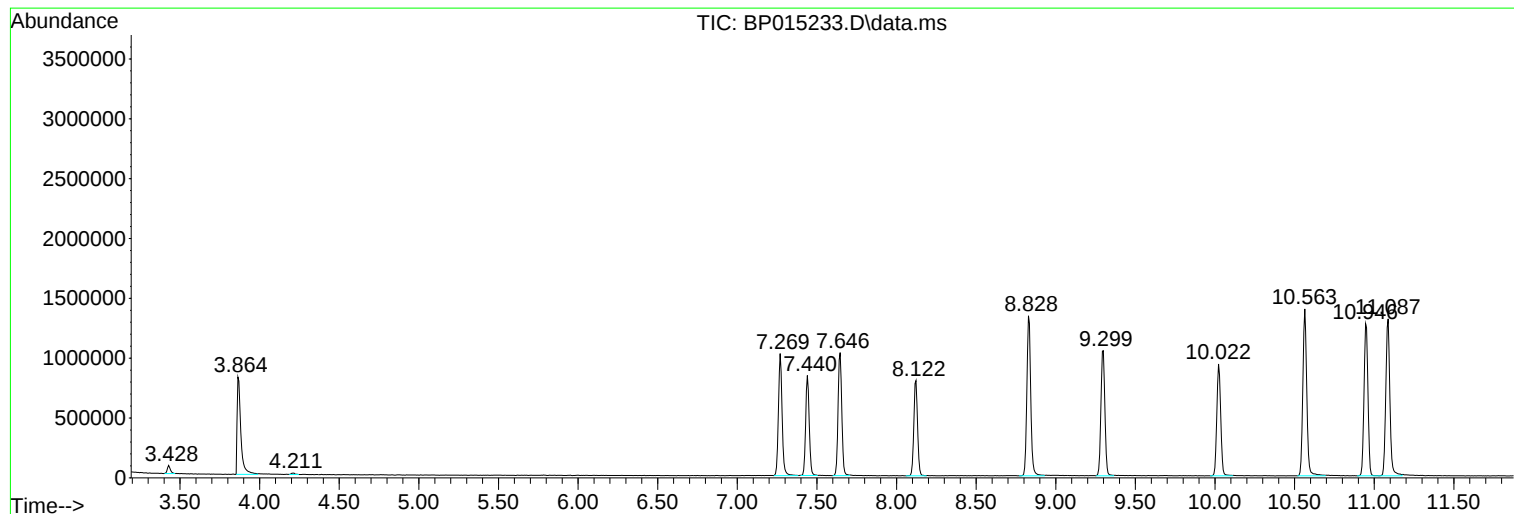

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015233.D
Acq On : 23 May 2023 10:56
Operator : CG/JU
Sample : PB152973BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015233.D
Acq On : 23 May 2023 10:56
Operator : CG/JU
Sample : PB152973BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK973

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------