

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015237.D
 Acq On : 23 May 2023 13:10
 Operator : CG/JU
 Sample : 02861-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	48	rVB	48415	65538	1.07%	0.112%
2	3.875	115	117	133	rBV	222462	374936	6.15%	0.640%
3	4.111	152	157	162	rVB	12829	19011	0.31%	0.032%
4	4.211	170	174	182	rVB3	12753	21317	0.35%	0.036%
5	4.669	247	252	258	rVB	18230	28249	0.46%	0.048%
6	5.287	350	357	362	rVB10	3655	7809	0.13%	0.013%
7	5.658	414	420	424	rVB5	4654	8133	0.13%	0.014%
8	5.781	436	441	445	rVB	8515	13277	0.22%	0.023%
9	7.222	681	686	689	rBV	12557	18310	0.30%	0.031%
10	7.269	689	694	704	rVB	181315	298995	4.90%	0.510%
11	7.440	715	723	735	rBV	817212	1279502	20.99%	2.183%
12	7.646	748	758	768	rBV	763329	1241225	20.36%	2.117%
13	7.722	768	771	779	rVB10	5655	10175	0.17%	0.017%
14	8.122	831	839	847	rBV	815330	1328941	21.80%	2.267%
15	8.828	952	959	973	rBV	581527	992542	16.28%	1.693%
16	9.299	1032	1039	1050	rBV	976285	1658944	27.21%	2.830%
17	9.399	1052	1056	1063	rVB8	4204	7777	0.13%	0.013%
18	9.687	1100	1105	1111	rVB	35646	55493	0.91%	0.095%
19	10.022	1153	1162	1176	rBV	806428	1364447	22.38%	2.328%
20	10.563	1245	1254	1269	rBV	1152084	1996092	32.74%	3.405%
21	10.951	1312	1320	1329	rBV	1189293	2033371	33.35%	3.469%
22	11.087	1335	1343	1360	rBV	984465	1789434	29.35%	3.053%
23	12.181	1524	1529	1534	rBV	27653	42434	0.70%	0.072%
24	12.528	1582	1588	1596	rBV3	18944	34720	0.57%	0.059%
25	12.745	1621	1625	1630	rBV7	3805	7086	0.12%	0.012%
26	13.363	1725	1730	1735	rBV9	4799	9651	0.16%	0.016%
27	13.563	1760	1764	1770	rVB9	6204	11623	0.19%	0.020%
28	13.645	1770	1778	1782	rBV3	18191	31478	0.52%	0.054%
29	14.163	1857	1866	1881	rBV	2569912	3568071	58.52%	6.087%
30	14.451	1908	1915	1931	rBV	2609943	4008981	65.75%	6.839%
31	14.757	1960	1967	1982	rVV	1927321	2834798	46.49%	4.836%
32	14.957	1994	2001	2016	rBV2	103131	238487	3.91%	0.407%
33	15.157	2032	2035	2041	rVB8	10476	16375	0.27%	0.028%
34	15.363	2059	2070	2073	rBV3	85554	257135	4.22%	0.439%
35	15.704	2124	2128	2130	rBV2	19980	26774	0.44%	0.046%
36	15.751	2130	2136	2149	rVB	3496726	5070958	83.17%	8.651%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015237.D
 Acq On : 23 May 2023 13:10
 Operator : CG/JU
 Sample : 02861-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.869	2150	2156	2168	rBV	1072356	1521353	24.95%	2.595%
38	15.986	2173	2176	2183	rVB3	18790	28456	0.47%	0.049%
39	16.110	2192	2197	2204	rBV	96619	132193	2.17%	0.226%
40	16.451	2252	2255	2258	rBV3	8499	9105	0.15%	0.016%
41	16.957	2337	2341	2345	rBV2	24356	34611	0.57%	0.059%
42	17.510	2429	2435	2443	rBV	2327916	3308475	54.26%	5.644%
43	17.610	2446	2452	2459	rVV	4023079	5682099	93.19%	9.693%
44	18.369	2577	2581	2590	rBV2	201265	298449	4.89%	0.509%
45	19.833	2824	2830	2836	rVB	4633094	6097114	100.00%	10.401%
46	21.269	3070	3074	3081	rBV4	125971	251558	4.13%	0.429%
47	21.586	3123	3128	3135	rBV	1954730	2667639	43.75%	4.551%
48	23.974	3527	3534	3547	rVB2	2437669	5229089	85.76%	8.920%
49	24.139	3556	3562	3572	rVB	1182513	2586711	42.43%	4.413%




Sum of corrected areas: 58618941

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015237.D
Acq On : 23 May 2023 13:10
Operator : CG/JU
Sample : 02861-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

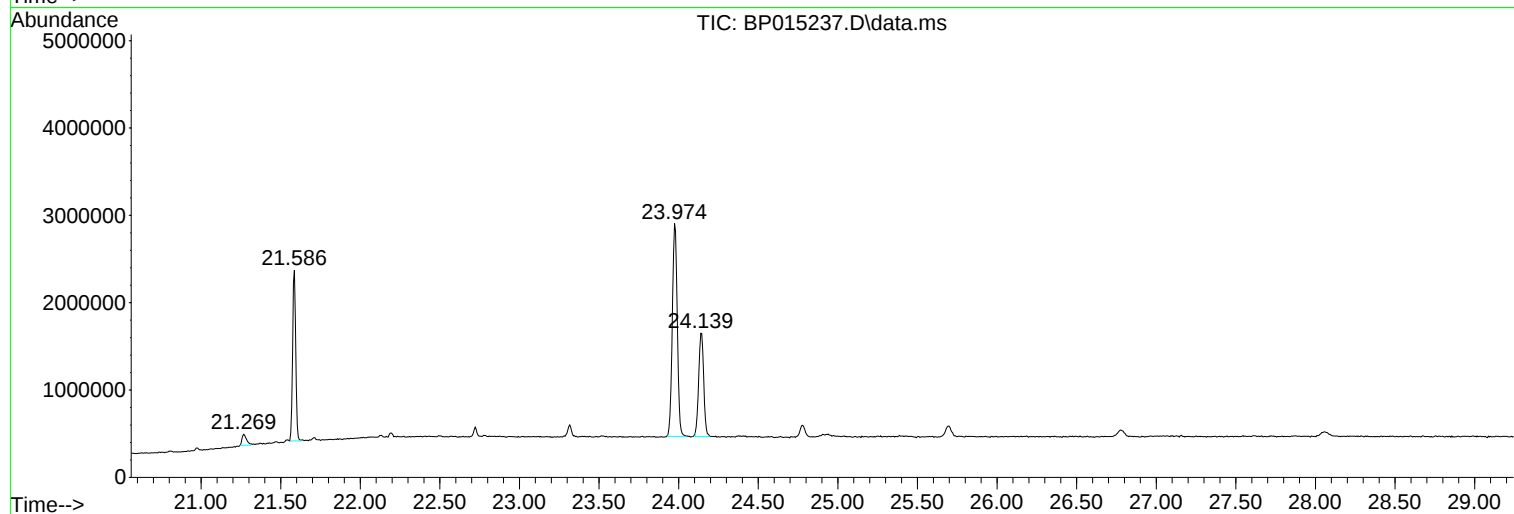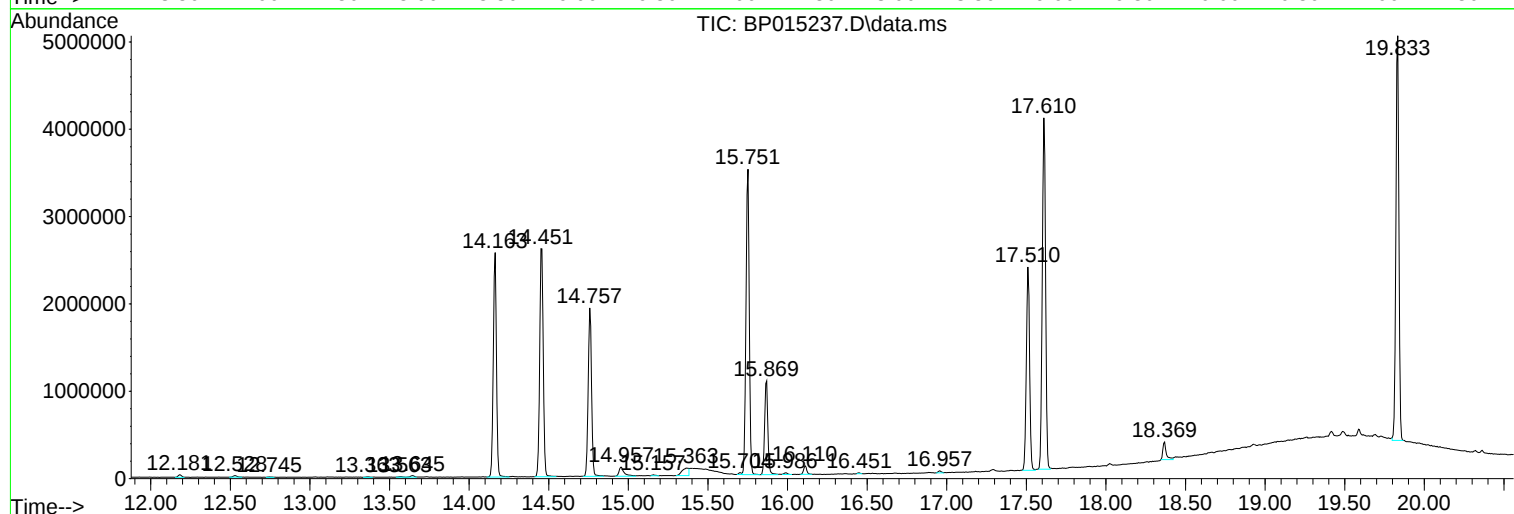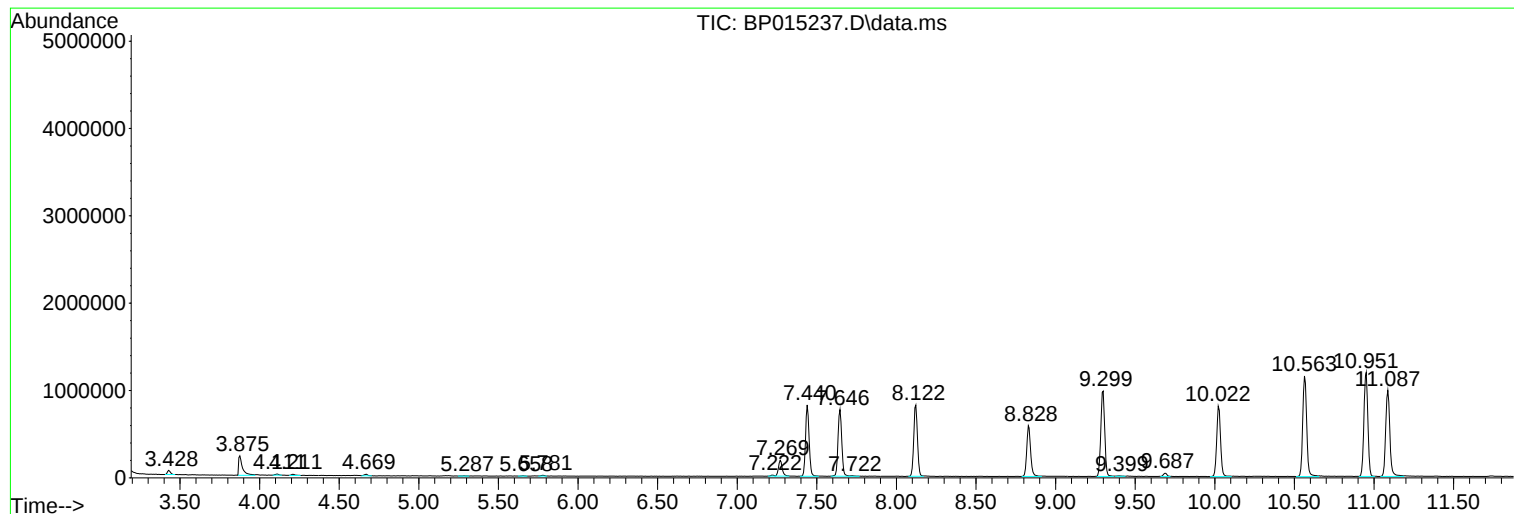

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015237.D
Acq On : 23 May 2023 13:10
Operator : CG/JU
Sample : 02861-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015237.D
Acq On : 23 May 2023 13:10
Operator : CG/JU
Sample : 02861-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc