

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015248.D
 Acq On : 23 May 2023 19:54
 Operator : CG/JU
 Sample : PB152975BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK975

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	53	rVB	75511	112782	1.99%	0.171%
2	3.864	113	115	141	rBV	910628	1447959	25.57%	2.190%
3	4.211	170	174	178	rVB	13692	17770	0.31%	0.027%
4	7.269	687	694	709	rBV	1097821	1811027	31.98%	2.739%
5	7.440	716	723	737	rVB	914628	1428820	25.23%	2.161%
6	7.640	750	757	770	rBV	1109006	1840181	32.50%	2.783%
7	8.116	831	838	847	rBV	855836	1415230	24.99%	2.140%
8	8.828	951	959	973	rBV	1445717	2399282	42.37%	3.629%
9	9.293	1030	1038	1048	rBV	1046247	1776387	31.37%	2.687%
10	10.022	1155	1162	1176	rBV	945568	1560527	27.56%	2.360%
11	10.563	1246	1254	1273	rBV	1386506	2384604	42.11%	3.606%
12	10.946	1309	1319	1327	rBV	1273276	2139387	37.78%	3.235%
13	11.081	1335	1342	1362	rBV	1350122	2429525	42.90%	3.674%
14	12.534	1583	1589	1599	rVB2	18155	39961	0.71%	0.060%
15	13.640	1773	1777	1783	rBV2	18802	29520	0.52%	0.045%
16	13.734	1788	1793	1797	rVV7	4282	6645	0.12%	0.010%
17	14.163	1858	1866	1877	rBV	2515895	3661159	64.65%	5.537%
18	14.281	1880	1886	1889	rVB6	3396	7649	0.14%	0.012%
19	14.451	1908	1915	1927	rBV	3036343	4409208	77.86%	6.668%
20	14.757	1960	1967	1978	rBV	2051576	3017874	53.29%	4.564%
21	14.945	1993	1999	2023	rBV	874089	1554623	27.45%	2.351%
22	15.169	2034	2037	2047	rVB	9384	15985	0.28%	0.024%
23	15.745	2128	2135	2148	rBV	3542269	5294259	93.49%	8.007%
24	15.863	2148	2155	2171	rVV	860948	1260935	22.27%	1.907%
25	15.987	2172	2176	2184	rVB3	18877	33397	0.59%	0.051%
26	16.316	2227	2232	2237	rBV9	3493	7921	0.14%	0.012%
27	16.534	2263	2269	2275	rVB9	4196	9114	0.16%	0.014%
28	17.181	2376	2379	2384	rVV7	5918	9451	0.17%	0.014%
29	17.298	2396	2399	2406	rVB5	6050	11194	0.20%	0.017%
30	17.510	2428	2435	2445	rBV	2407419	3491652	61.66%	5.281%
31	17.610	2445	2452	2466	rVV	3838567	5454217	96.32%	8.249%
32	19.404	2753	2757	2761	rBV	52234	72975	1.29%	0.110%
33	19.475	2765	2769	2776	rVB2	41517	66370	1.17%	0.100%
34	19.828	2823	2829	2839	rBV	4277423	5662831	100.00%	8.564%
35	21.586	3122	3128	3137	rBV	1927231	2891541	51.06%	4.373%
36	22.721	3318	3321	3328	rVB2	112488	165426	2.92%	0.250%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015248.D
Acq On : 23 May 2023 19:54
Operator : CG/JU
Sample : PB152975BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	23.316	3418	3422	3429	rVB2	166269	262160	4.63%	0.396%
38	23.974	3526	3534	3545	rBV2	2329524	5097980	90.03%	7.710%
39	24.139	3555	3562	3573	rVB	1315458	2825097	49.89%	4.273%




Sum of corrected areas: 66122625

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015248.D
Acq On : 23 May 2023 19:54
Operator : CG/JU
Sample : PB152975BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

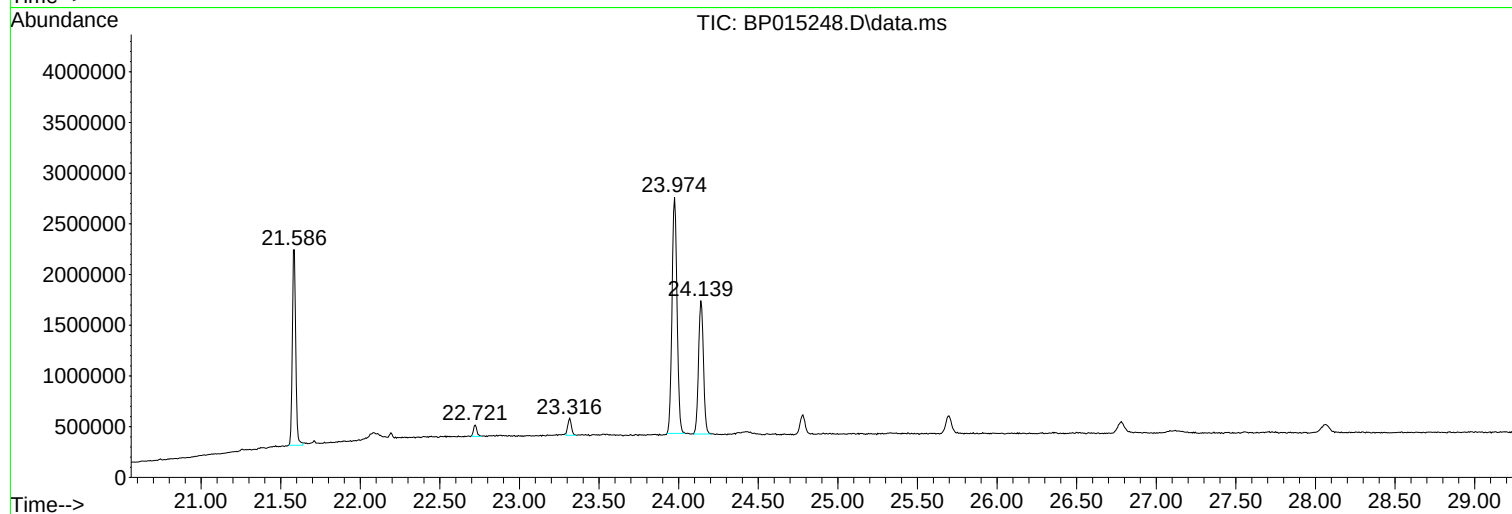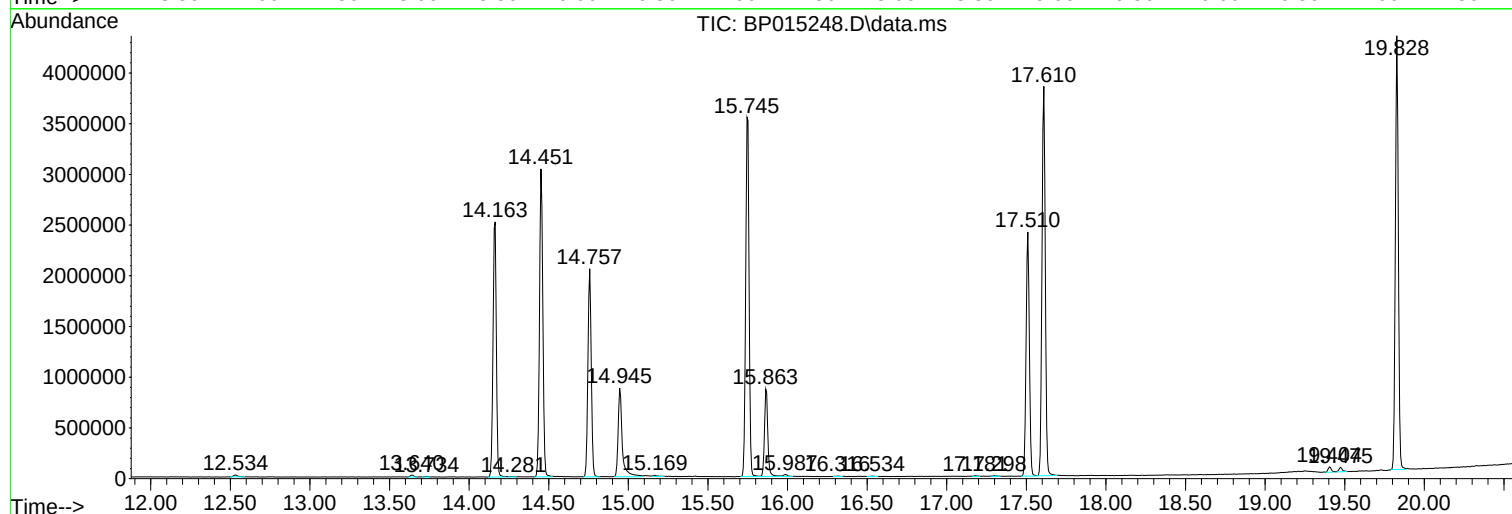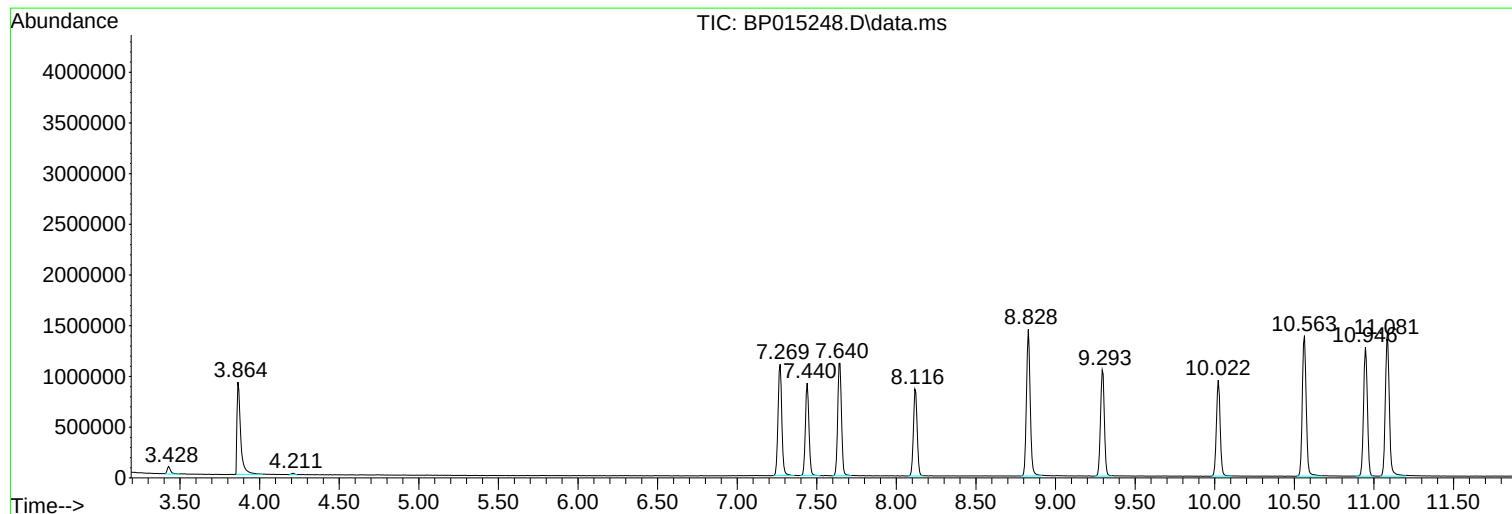

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015248.D
Acq On : 23 May 2023 19:54
Operator : CG/JU
Sample : PB152975BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015248.D
Acq On : 23 May 2023 19:54
Operator : CG/JU
Sample : PB152975BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK975

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------