

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015250.D
 Acq On : 23 May 2023 21:01
 Operator : CG/JU
 Sample : PB152979BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK979

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	8	10	18	rVB2	18436	23045	0.40%	0.035%
2	3.428	37	41	50	rVB	87260	119594	2.07%	0.179%
3	3.870	114	116	133	rBV	429019	683079	11.82%	1.023%
4	4.205	169	173	178	rBV	14646	21448	0.37%	0.032%
5	7.269	687	694	712	rVB	1196219	1938241	33.53%	2.903%
6	7.440	716	723	737	rVB	980596	1543158	26.69%	2.311%
7	7.640	750	757	770	rBV	1223764	1990262	34.43%	2.981%
8	8.116	830	838	849	rBV	969968	1539384	26.63%	2.305%
9	8.828	951	959	973	rBV	1562123	2528549	43.74%	3.787%
10	9.293	1031	1038	1053	rBV	1145509	1893426	32.75%	2.836%
11	10.022	1153	1162	1174	rBV	1007368	1663812	28.78%	2.492%
12	10.563	1246	1254	1275	rBV	1448104	2583854	44.69%	3.870%
13	10.946	1311	1319	1327	rBV	1400151	2305881	39.89%	3.453%
14	11.087	1335	1343	1362	rBV	415583	814910	14.10%	1.220%
15	12.534	1581	1589	1598	rBV2	20851	46602	0.81%	0.070%
16	13.640	1772	1777	1787	rBV	35586	60594	1.05%	0.091%
17	13.734	1790	1793	1799	rVB7	5074	9880	0.17%	0.015%
18	14.157	1859	1865	1874	rBV	2692934	3887100	67.24%	5.821%
19	14.451	1907	1915	1932	rBV	3105218	4702157	81.34%	7.042%
20	14.757	1960	1967	1976	rBV	2183820	3183255	55.06%	4.767%
21	14.946	1992	1999	2019	rBV	911543	1635064	28.28%	2.449%
22	15.163	2034	2036	2044	rVB9	6823	9118	0.16%	0.014%
23	15.751	2128	2136	2147	rBV	3843675	5580676	96.53%	8.358%
24	15.863	2149	2155	2167	rVV	934853	1343832	23.24%	2.012%
25	15.987	2172	2176	2182	rVB2	20095	31261	0.54%	0.047%
26	16.528	2264	2268	2273	rVB7	4036	7377	0.13%	0.011%
27	17.187	2376	2380	2385	rVB7	6905	10058	0.17%	0.015%
28	17.292	2394	2398	2405	rBV4	6124	11247	0.19%	0.017%
29	17.510	2428	2435	2445	rBV	2522193	3594398	62.17%	5.383%
30	17.610	2445	2452	2467	rBV2	3943643	5564512	96.25%	8.333%
31	19.404	2753	2757	2763	rVB2	47478	67307	1.16%	0.101%
32	19.475	2765	2769	2777	rVV	41553	60610	1.05%	0.091%
33	19.828	2823	2829	2839	rBV	4457899	5781172	100.00%	8.658%
34	21.586	3122	3128	3138	rBV	2148833	3037806	52.55%	4.549%
35	23.974	3526	3534	3546	rBV2	2513092	5393942	93.30%	8.078%
36	24.139	3555	3562	3576	rVB	1422749	3107692	53.76%	4.654%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015250.D
Acq On : 23 May 2023 21:01
Operator : CG/JU
Sample : PB152979BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 66774303

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015250.D
Acq On : 23 May 2023 21:01
Operator : CG/JU
Sample : PB152979BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

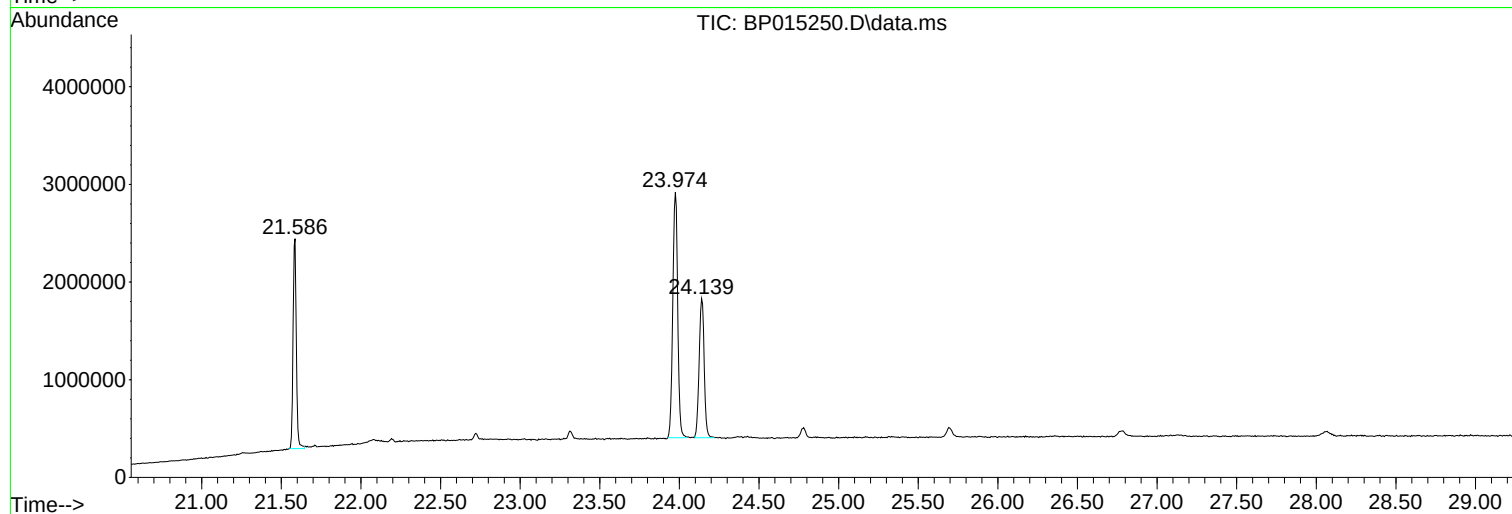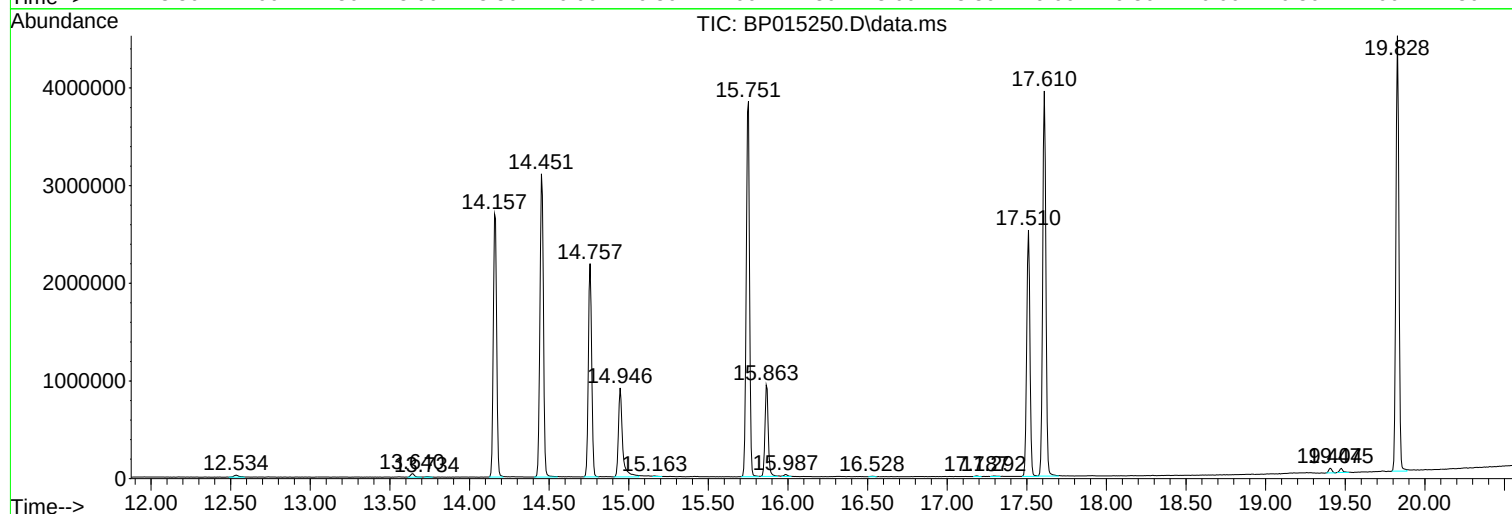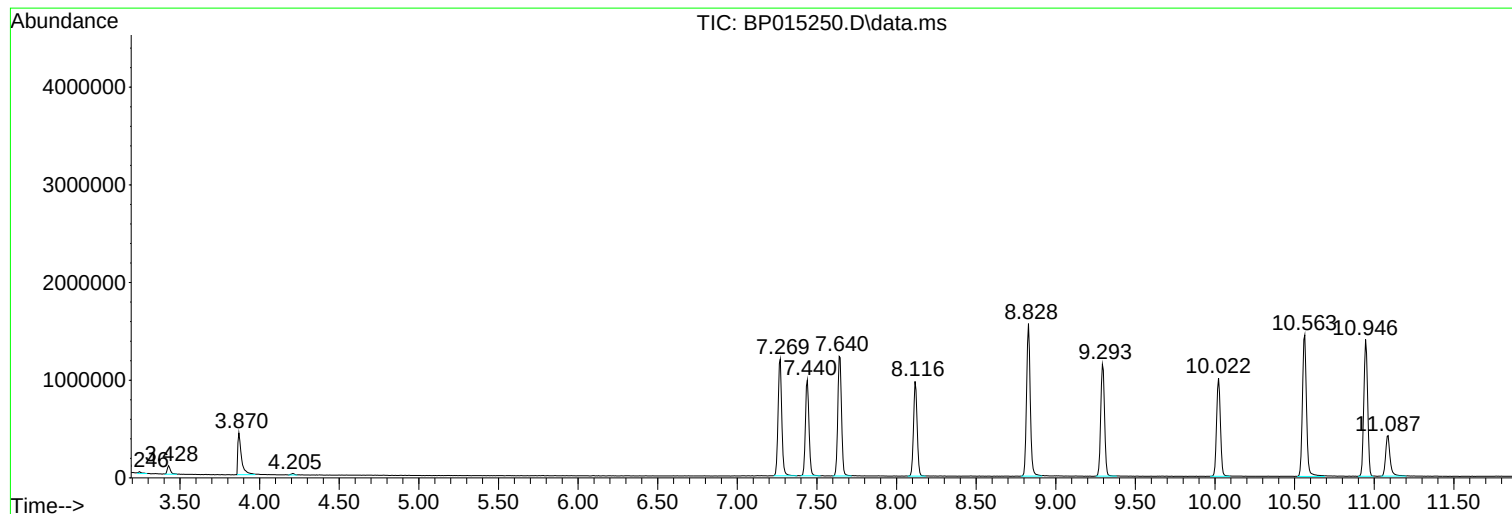

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015250.D
Acq On : 23 May 2023 21:01
Operator : CG/JU
Sample : PB152979BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015250.D
Acq On : 23 May 2023 21:01
Operator : CG/JU
Sample : PB152979BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK979

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------