

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015252.D
 Acq On : 23 May 2023 22:08
 Operator : CG/JU
 Sample : 02822-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	37	41	50	rVB	62042	85734	1.22%	0.120%
2	3.875	115	117	132	rBV	173363	300938	4.29%	0.422%
3	4.111	151	157	164	rVB2	23746	40719	0.58%	0.057%
4	4.211	169	174	179	rBV	20845	30108	0.43%	0.042%
5	4.593	236	239	243	rBV5	6536	9777	0.14%	0.014%
6	4.664	247	251	258	rVB	37330	53983	0.77%	0.076%
7	5.652	415	419	424	rVB	8663	12375	0.18%	0.017%
8	5.781	436	441	447	rVB	19700	30562	0.44%	0.043%
9	7.222	681	686	689	rBV	31054	48477	0.69%	0.068%
10	7.269	689	694	706	rVB	213095	351312	5.01%	0.492%
11	7.440	716	723	736	rBV	970206	1552050	22.13%	2.176%
12	7.640	750	757	768	rBV	878127	1458258	20.80%	2.044%
13	7.722	768	771	776	rVB5	4799	7919	0.11%	0.011%
14	7.940	803	808	812	rVB8	3498	7089	0.10%	0.010%
15	8.010	812	820	823	rBV9	3374	7774	0.11%	0.011%
16	8.116	829	838	846	rBV	1068128	1721104	24.54%	2.413%
17	8.828	951	959	975	rBV	709418	1202143	17.14%	1.685%
18	9.293	1030	1038	1051	rBV	1259225	2097217	29.91%	2.940%
19	9.687	1096	1105	1111	rBV	90789	139650	1.99%	0.196%
20	10.022	1153	1162	1177	rBV	1000110	1684214	24.02%	2.361%
21	10.563	1245	1254	1278	rBV	1376536	2428703	34.63%	3.405%
22	10.946	1311	1319	1332	rBV	1576957	2642550	37.68%	3.704%
23	11.081	1335	1342	1359	rBV	1212092	2233004	31.84%	3.130%
24	12.181	1524	1529	1536	rVB	64540	92151	1.31%	0.129%
25	12.528	1582	1588	1597	rBV2	21671	44777	0.64%	0.063%
26	12.740	1621	1624	1632	rVB8	3119	7514	0.11%	0.011%
27	13.640	1772	1777	1786	rBV2	41857	68467	0.98%	0.096%
28	13.734	1790	1793	1799	rVB6	4646	8408	0.12%	0.012%
29	14.157	1858	1865	1880	rBV	3020422	4358835	62.16%	6.110%
30	14.451	1907	1915	1934	rBV	3378536	5035470	71.81%	7.059%
31	14.757	1960	1967	1978	rBV	2486695	3589309	51.18%	5.031%
32	14.951	1992	2000	2018	rBV	104738	252879	3.61%	0.354%
33	15.169	2031	2037	2045	rVB	12032	24783	0.35%	0.035%
34	15.486	2087	2091	2096	rBV	9919	14427	0.21%	0.020%
35	15.698	2121	2127	2130	rBV	49356	73303	1.05%	0.103%
36	15.745	2130	2135	2147	rVV	4279145	6255415	89.20%	8.769%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015252.D
 Acq On : 23 May 2023 22:08
 Operator : CG/JU
 Sample : 02822-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONQ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	15.863	2149	2155	2169	rVV	1122429	1596605	22.77%	2.238%
38	15.986	2172	2176	2181	rVB2	21942	32813	0.47%	0.046%
39	16.110	2191	2197	2202	rBV	233308	318731	4.55%	0.447%
40	16.439	2245	2253	2257	rBV8	8273	24012	0.34%	0.034%
41	16.533	2264	2269	2273	rVB7	6661	12276	0.18%	0.017%
42	16.675	2289	2293	2300	rVB2	18661	31887	0.45%	0.045%
43	16.951	2336	2340	2347	rVB	44333	60908	0.87%	0.085%
44	17.186	2375	2380	2385	rVB7	6489	10897	0.16%	0.015%
45	17.298	2395	2399	2408	rVB5	7357	15497	0.22%	0.022%
46	17.510	2427	2435	2444	rBV	2913422	4104749	58.53%	5.754%
47	17.610	2445	2452	2464	rBV	4758695	6705245	95.62%	9.399%
48	18.022	2517	2522	2526	rBV	39076	47135	0.67%	0.066%
49	18.363	2576	2580	2590	rBV	62245	92807	1.32%	0.130%
50	18.922	2672	2675	2680	rVB2	35464	45675	0.65%	0.064%
51	19.404	2753	2757	2762	rBV	65399	82900	1.18%	0.116%
52	19.475	2765	2769	2777	rVB	54448	81441	1.16%	0.114%
53	19.586	2785	2788	2792	rBV4	37716	49815	0.71%	0.070%
54	19.686	2802	2805	2809	rBV2	39724	47759	0.68%	0.067%
55	19.827	2823	2829	2840	rBV	5243921	7012532	100.00%	9.830%
56	20.363	2917	2920	2923	rBV	40766	42685	0.61%	0.060%
57	20.974	3021	3024	3029	rVB3	41085	48864	0.70%	0.068%
58	21.586	3122	3128	3138	rBV	2404469	3304648	47.12%	4.632%
59	23.974	3526	3534	3549	rVB2	2983657	6254108	89.18%	8.767%
60	24.139	3555	3562	3572	rVB	1629853	3342537	47.67%	4.685%




Sum of corrected areas: 71337924

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015252.D
Acq On : 23 May 2023 22:08
Operator : CG/JU
Sample : 02822-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

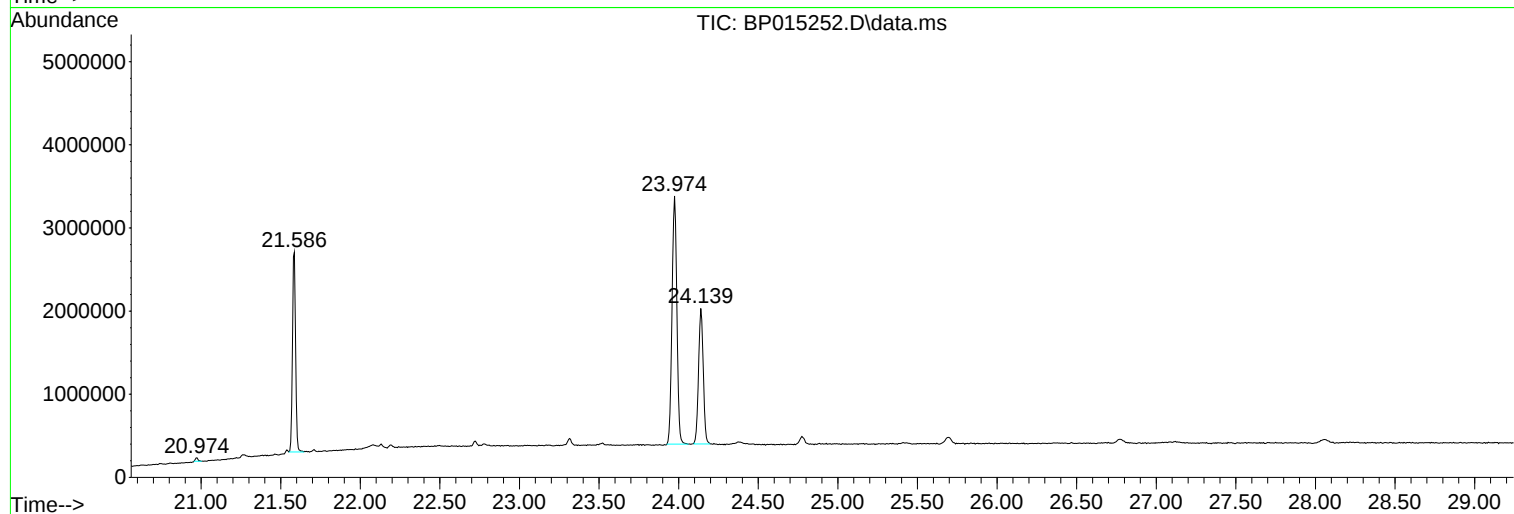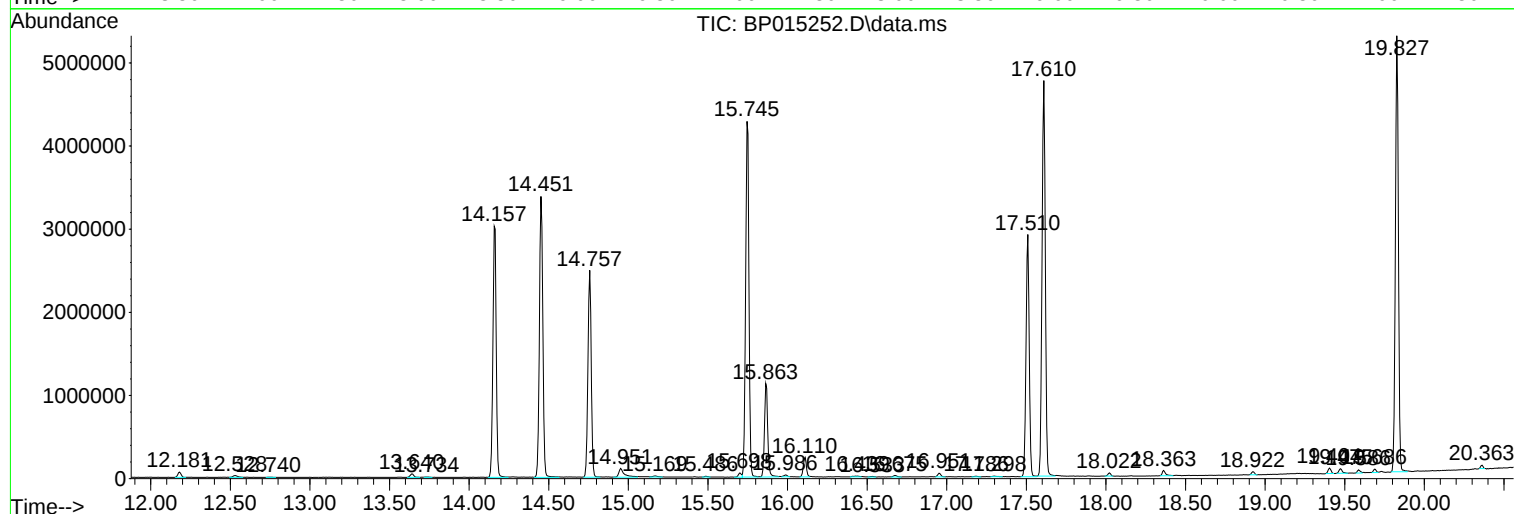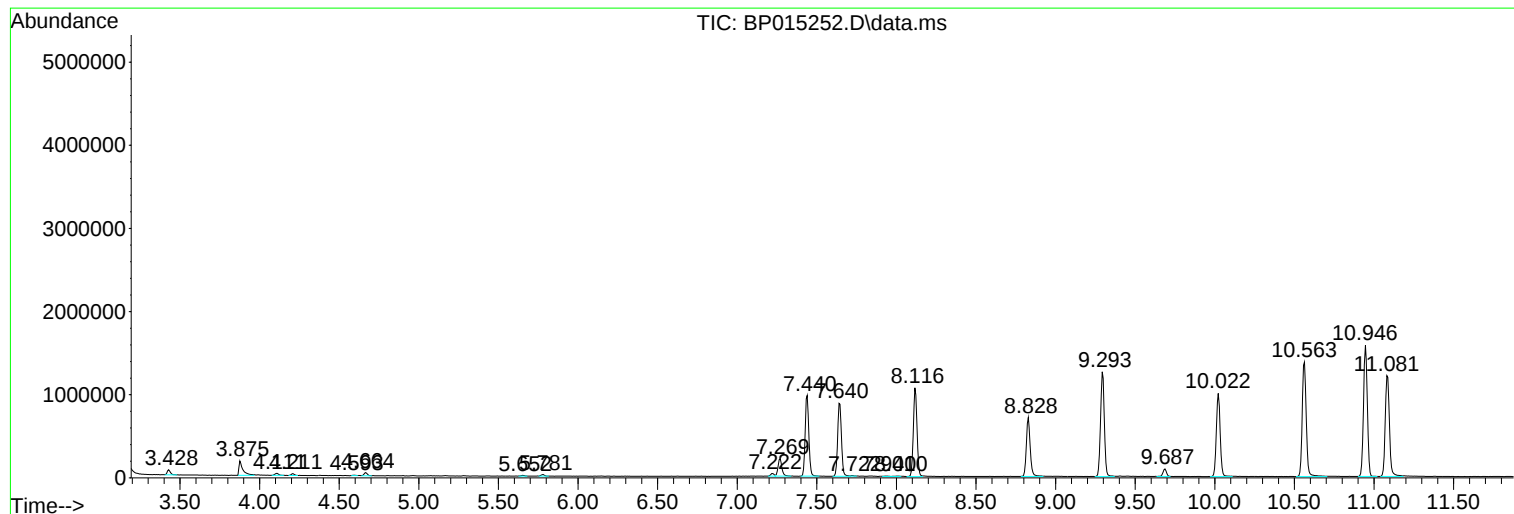

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015252.D
Acq On : 23 May 2023 22:08
Operator : CG/JU
Sample : 02822-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015252.D
Acq On : 23 May 2023 22:08
Operator : CG/JU
Sample : 02822-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
