

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
 Data File : BP015267.D
 Acq On : 24 May 2023 09:08
 Operator : CG/JU
 Sample : PB152989BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK989

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	37	40	49	rVB	66342	89559	1.75%	0.151%
2	3.864	111	115	139	rBV	716912	1183150	23.14%	1.990%
3	4.205	169	173	177	rVB3	11311	15768	0.31%	0.027%
4	5.769	435	439	443	rVB7	4567	7603	0.15%	0.013%
5	7.263	684	693	705	rBV	1044083	1680507	32.87%	2.826%
6	7.434	716	722	734	rVB	865528	1315655	25.73%	2.213%
7	7.640	750	757	771	rVB	1061105	1685218	32.96%	2.834%
8	8.116	829	838	851	rBV	798241	1273553	24.91%	2.142%
9	8.828	951	959	982	rBV	1347740	2207763	43.18%	3.713%
10	9.293	1030	1038	1047	rBV	1077868	1724080	33.72%	2.899%
11	10.022	1154	1162	1175	rBV	916669	1512809	29.59%	2.544%
12	10.563	1244	1254	1275	rBV	1331633	2301883	45.02%	3.871%
13	10.946	1309	1319	1329	rVB	1166213	1968611	38.51%	3.311%
14	11.087	1332	1343	1362	rBV	1160912	2105492	41.18%	3.541%
15	12.528	1583	1588	1595	rBV2	20731	36212	0.71%	0.061%
16	13.645	1770	1778	1784	rBV3	25379	45037	0.88%	0.076%
17	13.734	1787	1793	1800	rVV3	3961	9097	0.18%	0.015%
18	14.163	1860	1866	1881	rVB	2430623	3400762	66.52%	5.719%
19	14.457	1909	1916	1929	rBV	2708177	4006050	78.36%	6.737%
20	14.763	1961	1968	1979	rVB	1850824	2688664	52.59%	4.522%
21	14.951	1993	2000	2026	rBV	780417	1416076	27.70%	2.381%
22	15.163	2034	2036	2042	rVB7	5788	8739	0.17%	0.015%
23	15.428	2077	2081	2084	rVB5	4199	5523	0.11%	0.009%
24	15.504	2088	2094	2096	rBV7	3592	7824	0.15%	0.013%
25	15.698	2121	2127	2130	rBV7	8404	17276	0.34%	0.029%
26	15.757	2130	2137	2150	rVV	3271251	4830921	94.49%	8.124%
27	15.869	2150	2156	2170	rVV	826682	1186377	23.20%	1.995%
28	15.992	2173	2177	2183	rVB3	16716	27209	0.53%	0.046%
29	16.134	2197	2201	2207	rVB6	7042	10594	0.21%	0.018%
30	16.292	2225	2228	2231	rBV5	5811	8869	0.17%	0.015%
31	16.539	2267	2270	2276	rVB7	5386	7697	0.15%	0.013%
32	16.845	2318	2322	2326	rBV6	3893	5778	0.11%	0.010%
33	16.957	2337	2341	2344	rBV4	7579	9819	0.19%	0.017%
34	17.316	2397	2402	2405	rBV5	6192	11549	0.23%	0.019%
35	17.516	2429	2436	2446	rBV	2205569	3106982	60.77%	5.225%
36	17.616	2446	2453	2467	rVV2	3437324	4947915	96.78%	8.321%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015267.D
Acq On : 24 May 2023 09:08
Operator : CG/JU
Sample : PB152989BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK989

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	17.875	2495	2497	2500	rBV4	4726	6498	0.13%	0.011%
38	18.028	2520	2523	2529	rBV5	8361	13498	0.26%	0.023%
39	18.163	2544	2546	2549	rVB4	7052	6048	0.12%	0.010%
40	18.375	2580	2582	2584	rVB3	6275	5272	0.10%	0.009%
41	18.933	2674	2677	2681	rBV5	7345	8957	0.18%	0.015%
42	19.416	2755	2759	2763	rVB2	44482	58571	1.15%	0.099%
43	19.480	2766	2770	2779	rVV2	35702	66678	1.30%	0.112%
44	19.839	2825	2831	2843	rBV	3865369	5112595	100.00%	8.598%
45	21.592	3124	3129	3138	rBV	1783672	2527660	49.44%	4.251%
46	23.992	3529	3537	3553	rVB2	1982055	4359118	85.26%	7.331%
47	24.157	3558	3565	3576	rVB	1116816	2431350	47.56%	4.089%




Sum of corrected areas: 59462866

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015267.D
Acq On : 24 May 2023 09:08
Operator : CG/JU
Sample : PB152989BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

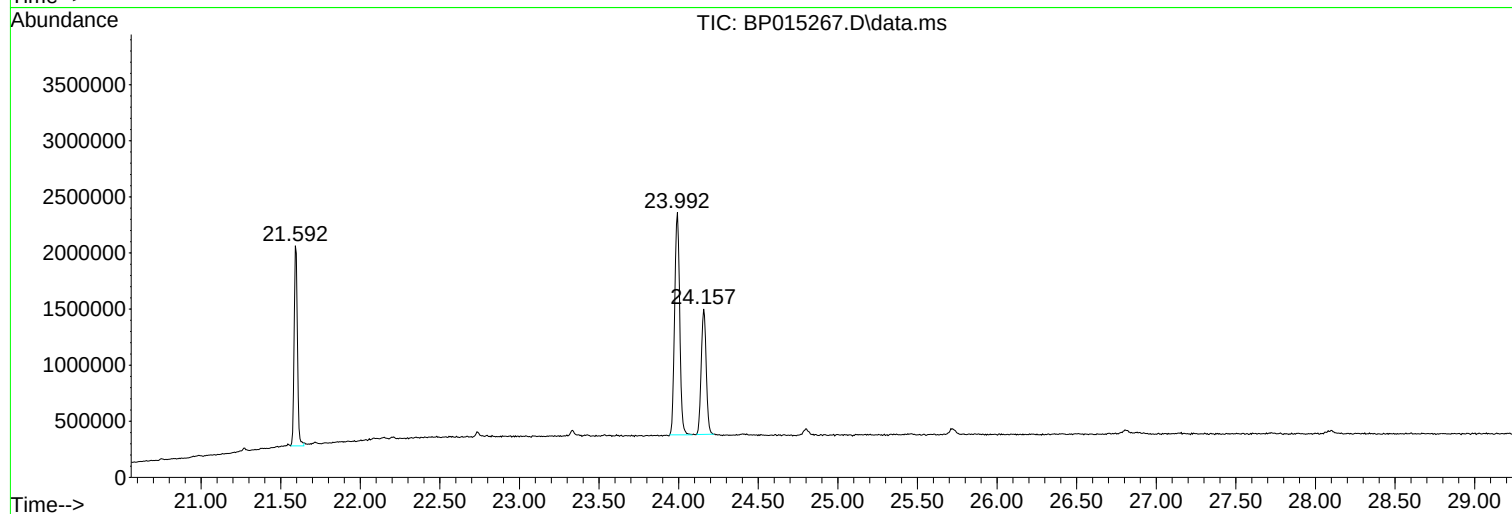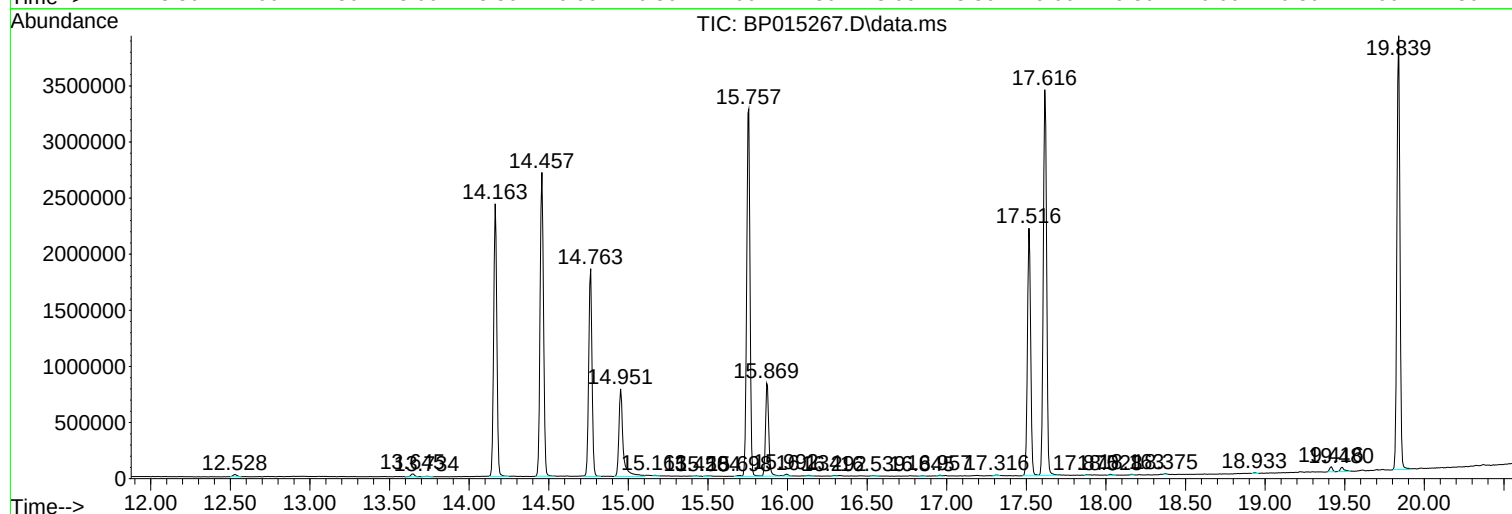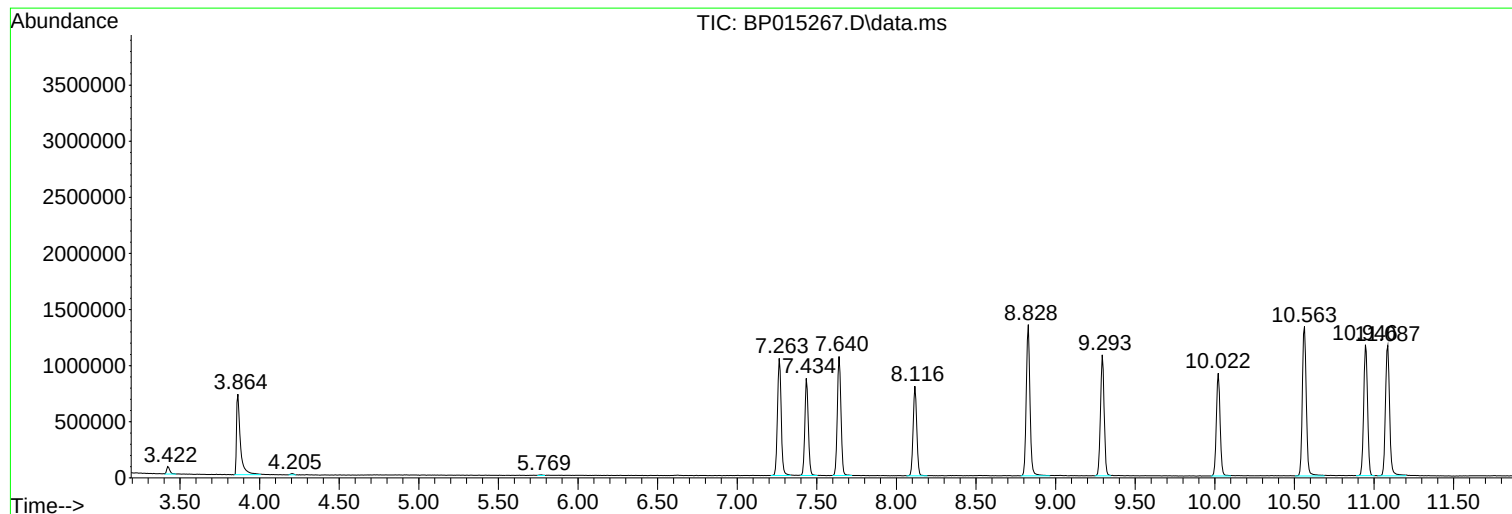

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015267.D
Acq On : 24 May 2023 09:08
Operator : CG/JU
Sample : PB152989BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052323\
Data File : BP015267.D
Acq On : 24 May 2023 09:08
Operator : CG/JU
Sample : PB152989BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------