
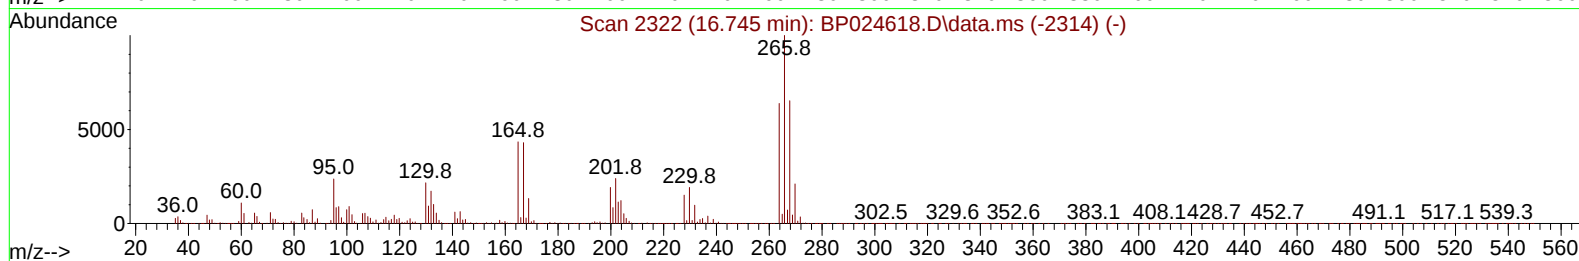
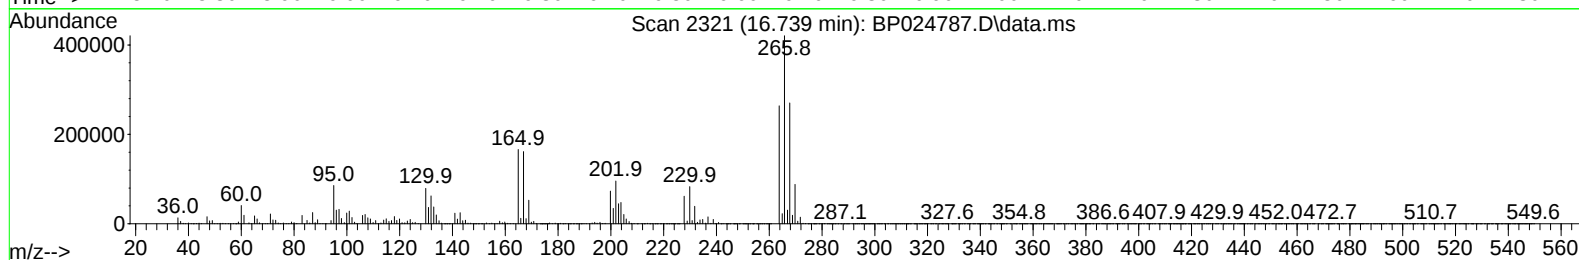


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052325\
Data File : BP024787.D
Acq On : 23 May 2025 10:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 23 12:13:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

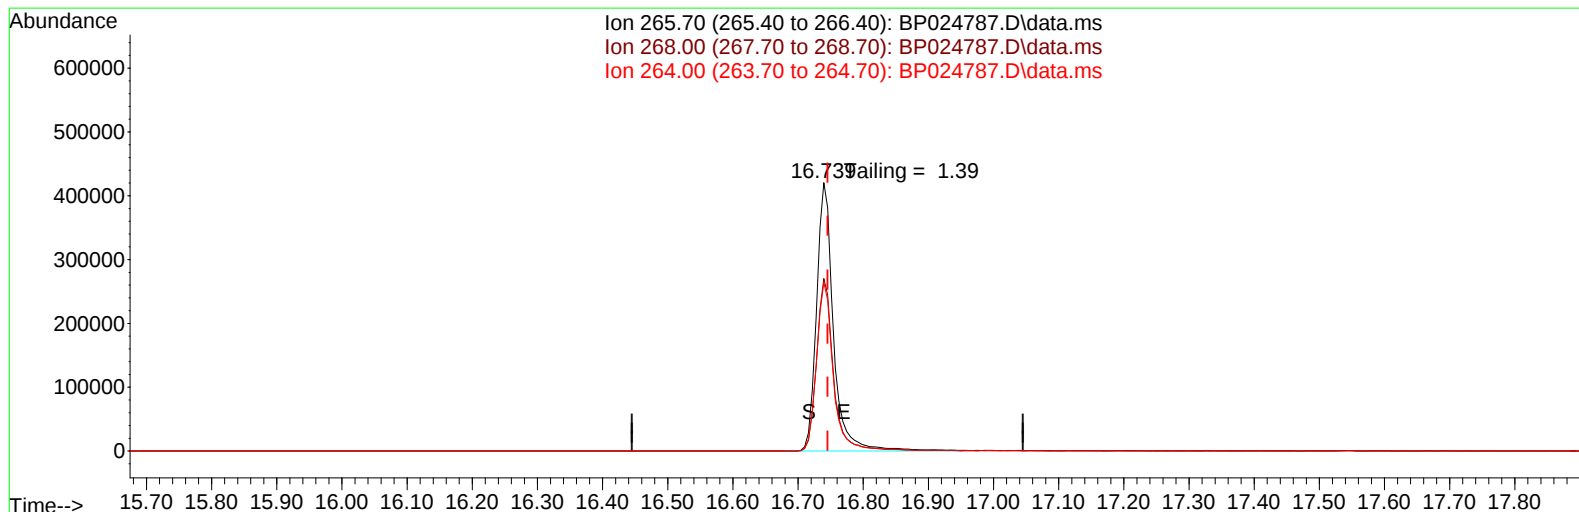

TIC: BP024787.D\data.ms

(70) Pentachlorophenol (C)




16.739min (-0.006) 1289316.61 ng

response 758576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.26
264.00	63.90	62.71
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052325\  
Data File : BP024787.D  
Acq On    : 23 May 2025  10:59  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 23 12:13:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

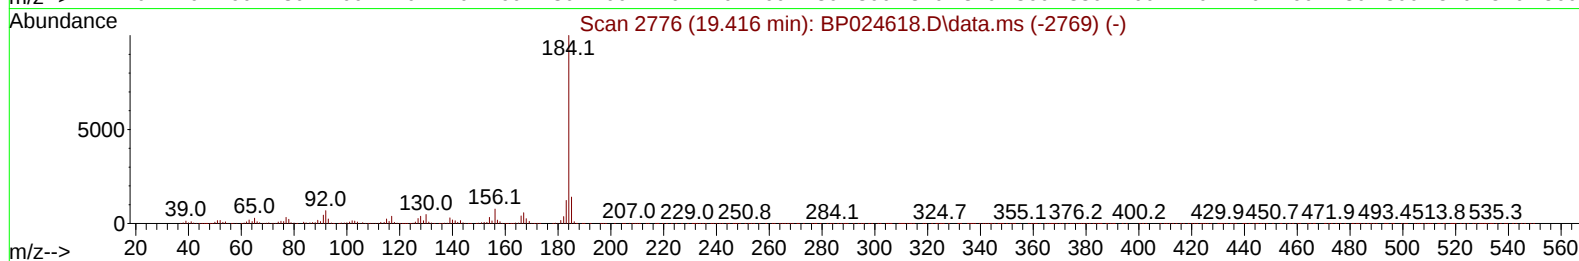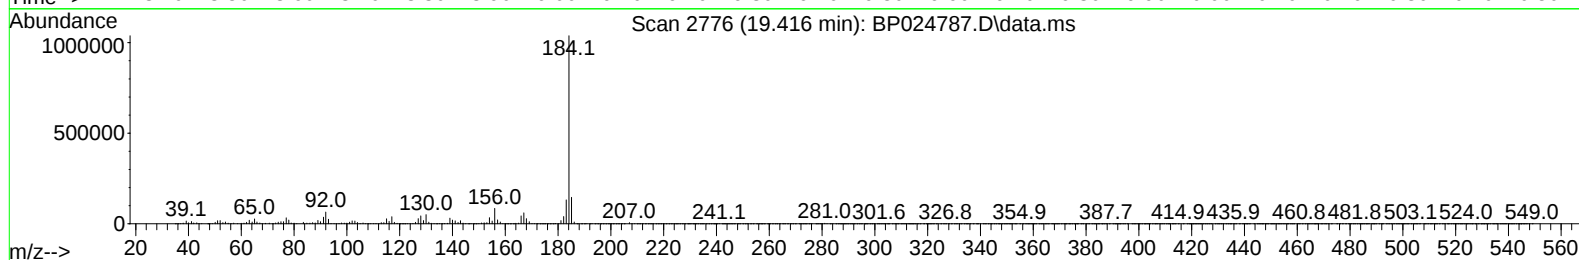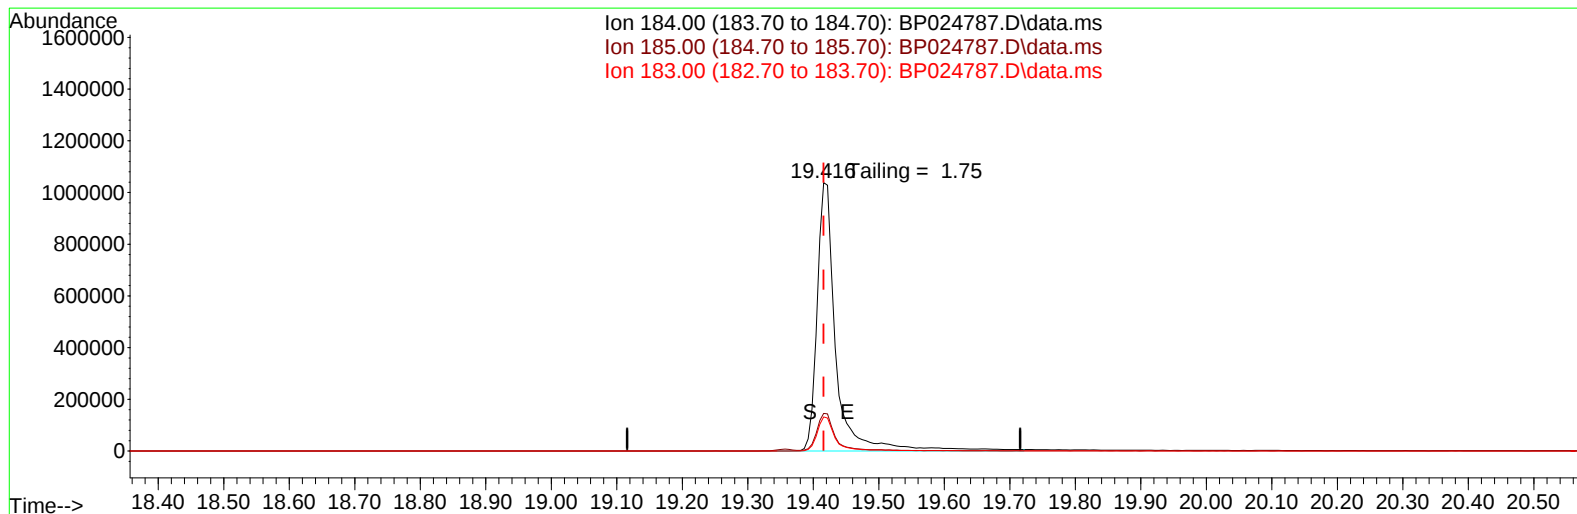

TIC: BP024787.D\data.ms

(77) Benzidine

19.416min (-0.000) 1952689.30 ng

response 2020967

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.00	14.02
--------	-------	-------

183.00	12.30	12.71
--------	-------	-------

0.00 0.00 0.00