
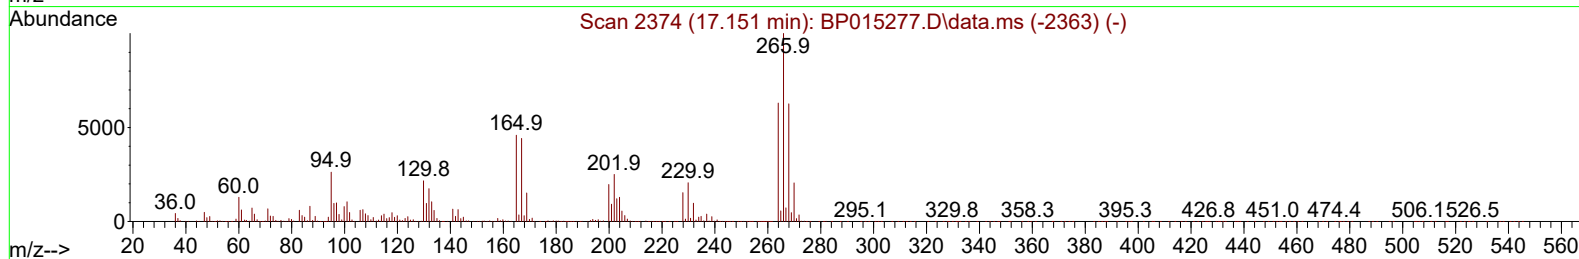
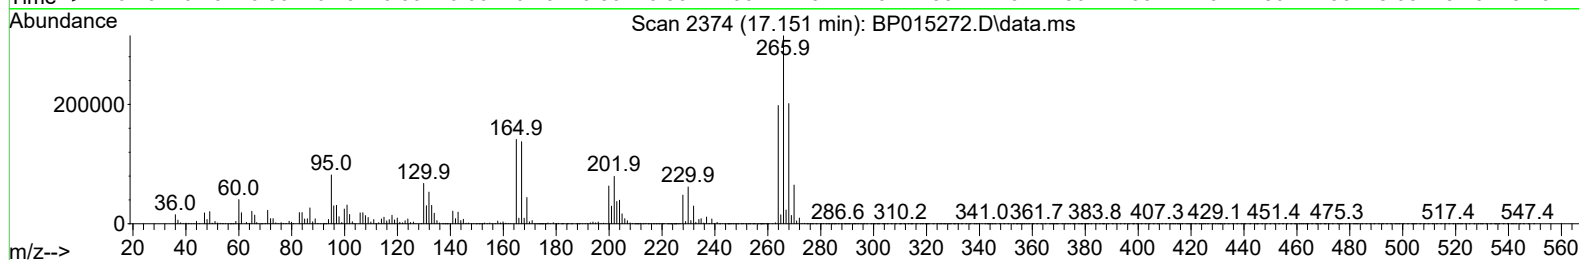


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015272.D
 Acq On : 24 May 2023 14:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:06:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

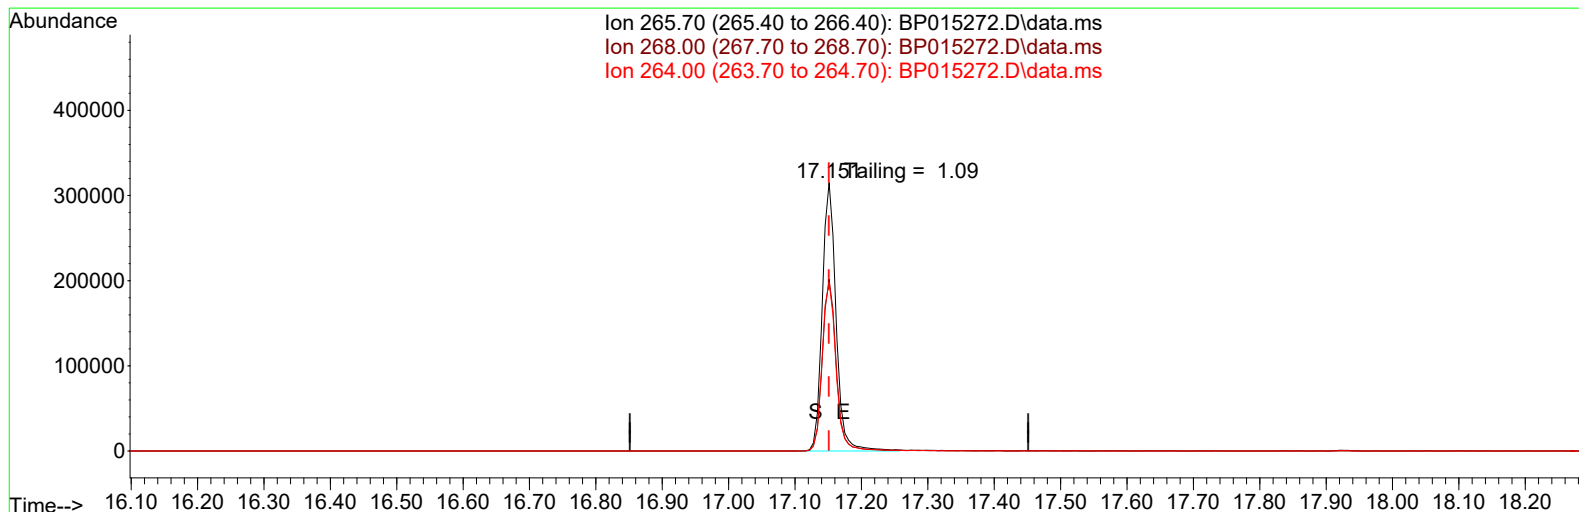

TIC: BP015272.D\data.ms

(70) Pentachlorophenol (C)




17.151min (+ 0.000) 847485.04 ng

response 456440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.89
264.00	63.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015272.D
 Acq On : 24 May 2023 14:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 25 07:06:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

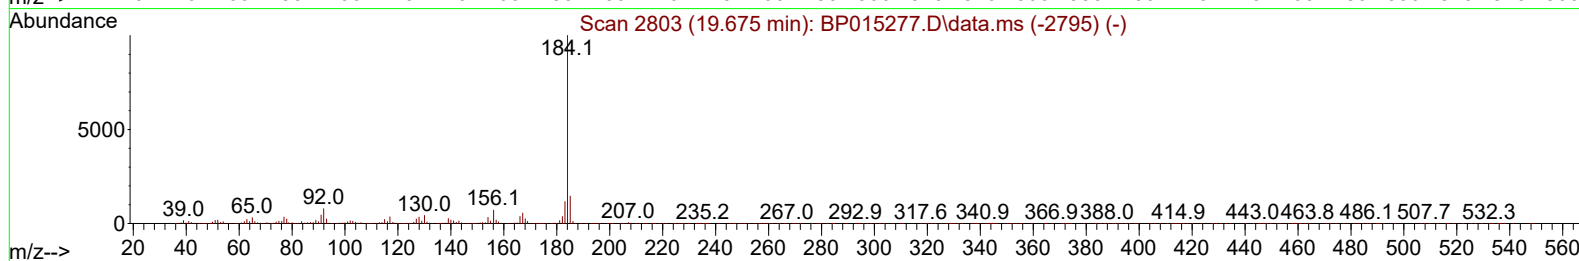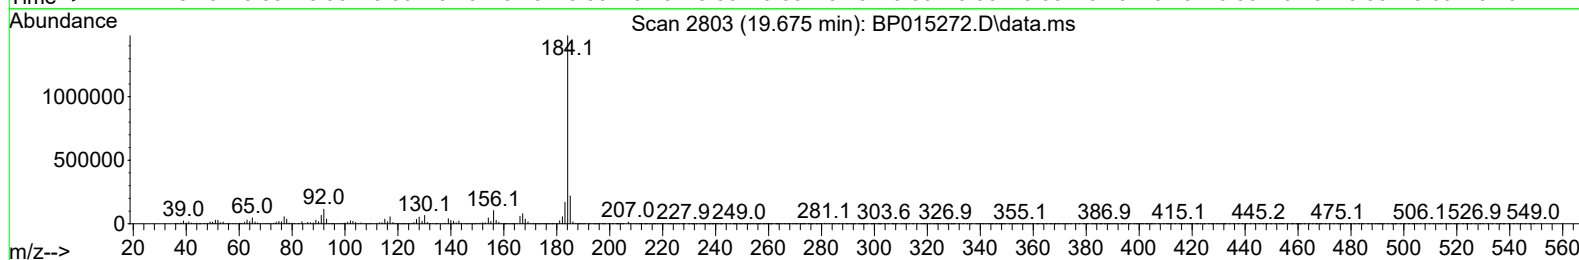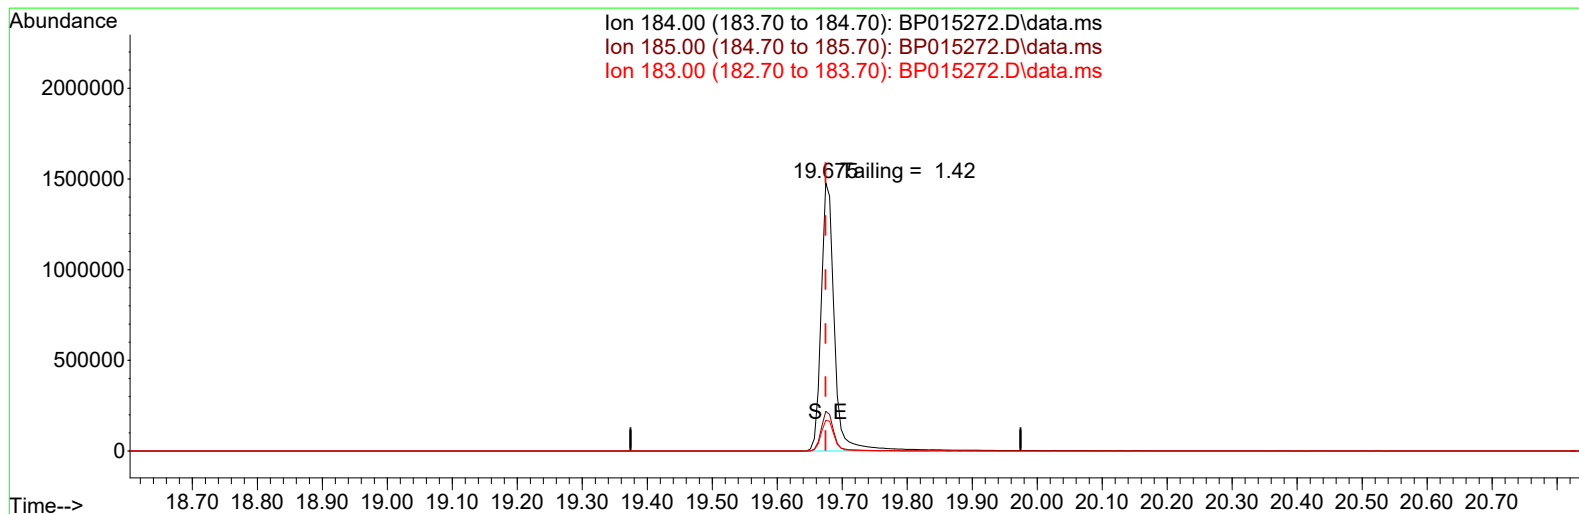

TIC: BP015272.D\data.ms

(77) Benzidine**19.675min (+ 0.000) 1094623.71 ng****response 2097378**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.79
183.00	11.70	11.46
0.00	0.00	0.00