

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015282.D
 Acq On : 24 May 2023 21:09
 Operator : CG/JU
 Sample : PB152920BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB152920BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP015282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.169	331	337	346	rBV	277421	386019	3.61%	0.643%
2	5.640	410	417	430	rBV	4945088	7200234	67.34%	12.002%
3	7.269	682	694	705	rBV	4295399	7237421	67.69%	12.064%
4	8.110	829	837	847	rBV	962201	1496933	14.00%	2.495%
5	9.287	1028	1037	1058	rBV	2737652	4778944	44.70%	7.966%
6	10.940	1308	1318	1328	rBV	1107965	1914057	17.90%	3.191%
7	13.375	1725	1732	1754	rBV	6475714	9972846	93.28%	16.624%
8	14.751	1958	1966	1982	rBV	1591466	2357295	22.05%	3.929%
9	16.239	2212	2219	2242	rBV	4981939	7234955	67.67%	12.060%
10	17.504	2427	2434	2449	rBV	1743839	2564399	23.98%	4.275%
11	20.039	2859	2865	2875	rBV	8797762	10691869	100.00%	17.822%
12	21.580	3122	3127	3137	rBV	1548704	2098420	19.63%	3.498%
13	24.133	3554	3561	3573	rVB	959400	2057856	19.25%	3.430%




Sum of corrected areas: 59991248

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
Data File : BP015282.D
Acq On : 24 May 2023 21:09
Operator : CG/JU
Sample : PB152920BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB152920BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

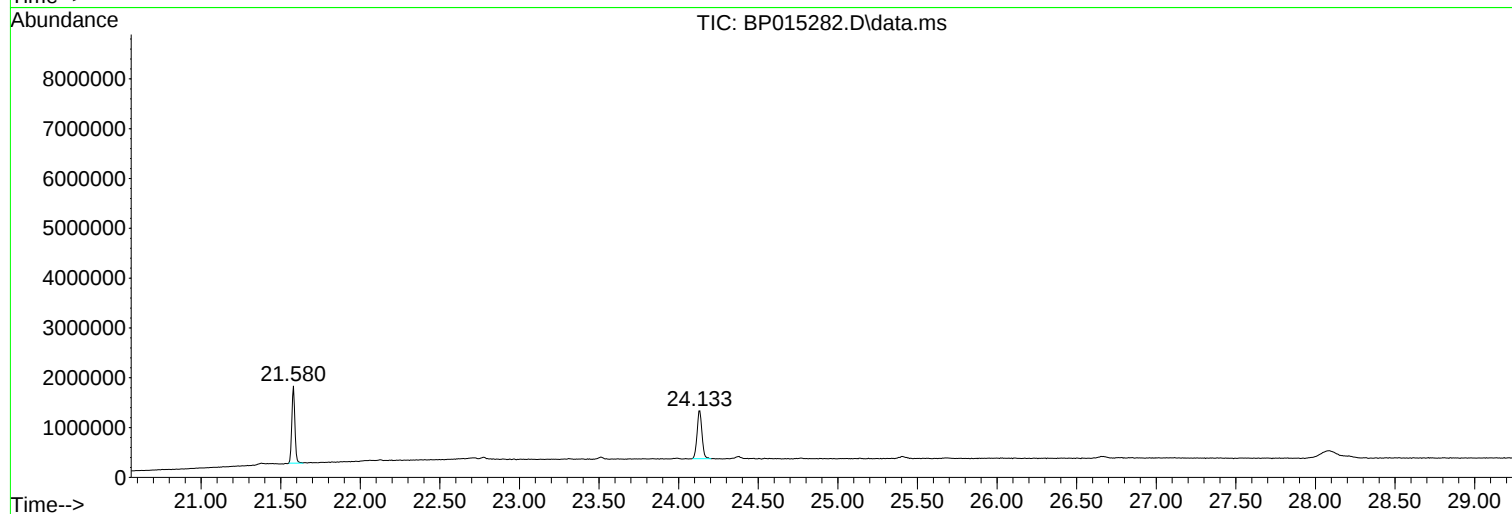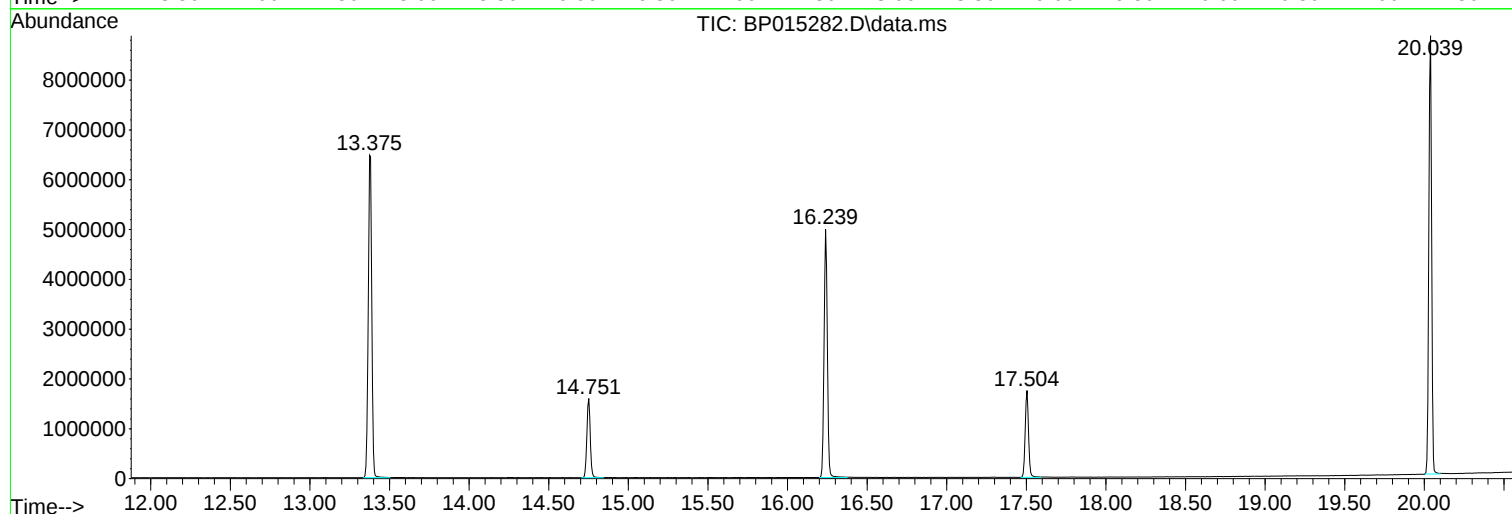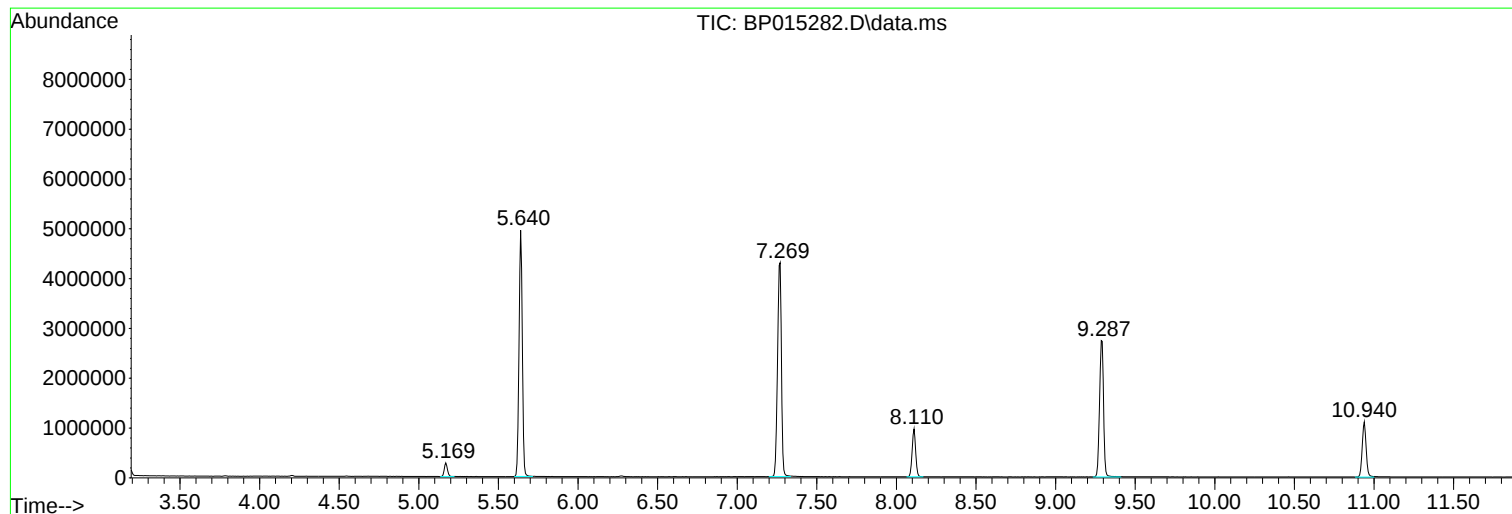

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
Data File : BP015282.D
Acq On : 24 May 2023 21:09
Operator : CG/JU
Sample : PB152920BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB152920BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.169	5.16 ng	386019	1,4-Dichlorobenzene-d4	8.110

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
3			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
5			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10

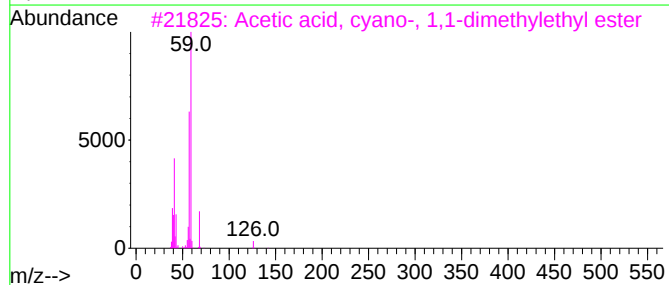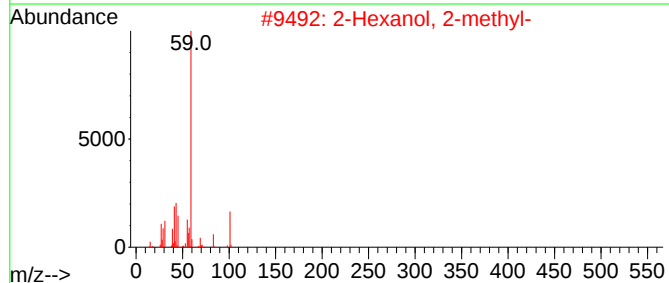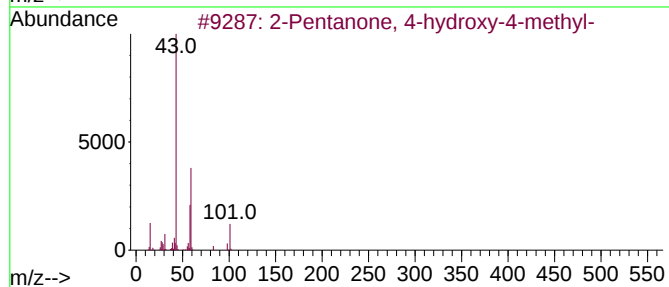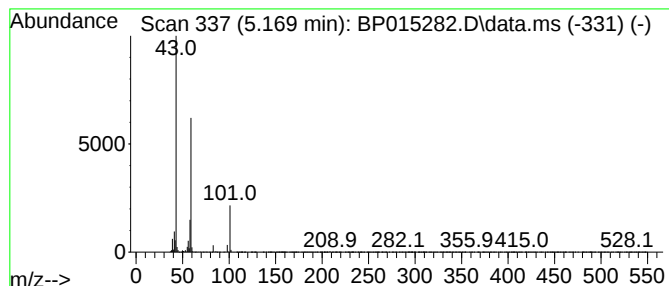

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
Data File : BP015282.D
Acq On : 24 May 2023 21:09
Operator : CG/JU
Sample : PB152920BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB152920BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.169	5.2	ng	386019	1	8.110	1496930	20.0