
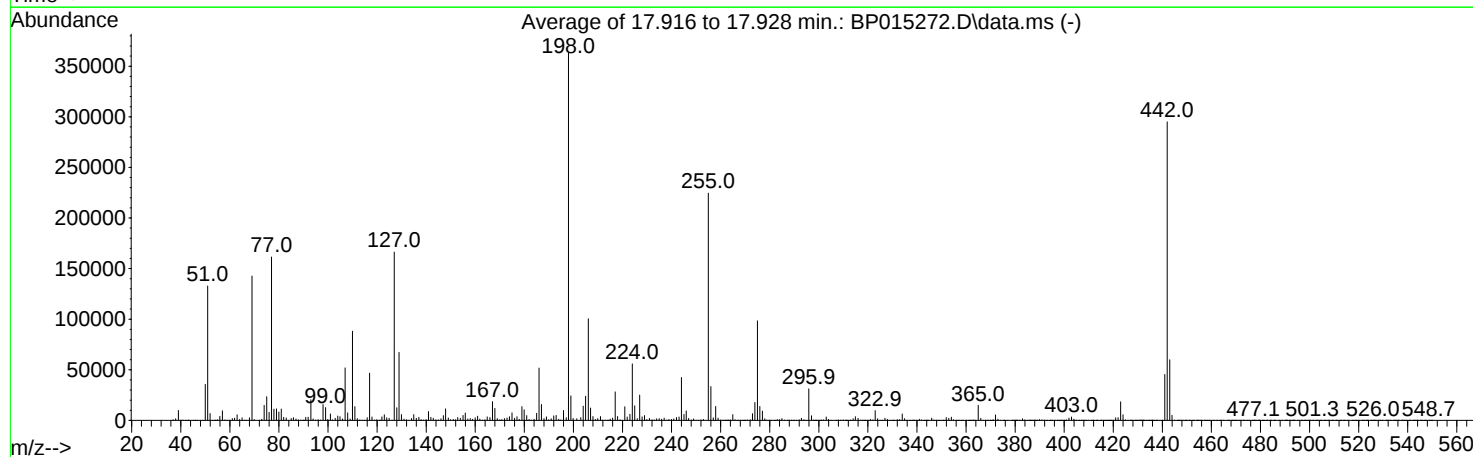


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015272.D
 Acq On : 24 May 2023 14:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 25 01:41:43 2023

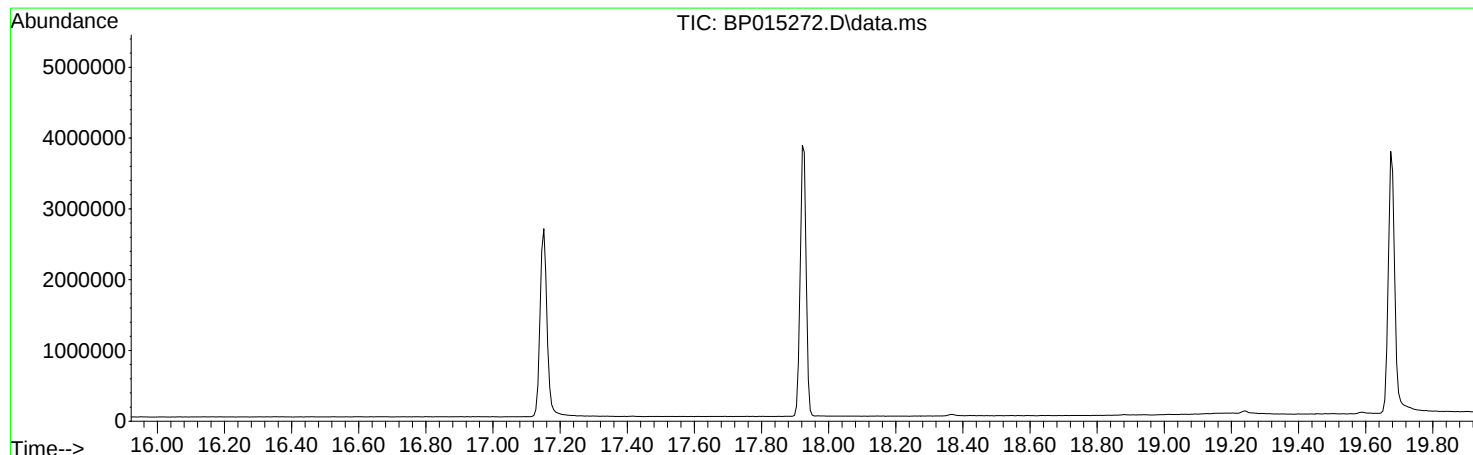

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	132894	PASS
68	69	0.00	2	1.8	2549	PASS
69	198	0.00	100	39.2	142665	PASS
70	69	0.00	2	0.5	735	PASS
127	198	10	80	45.7	166291	PASS
197	198	0.00	2	0.7	2682	PASS
198	198	100	100	100.0	363537	PASS
199	198	5	9	6.7	24210	PASS
275	198	10	60	27.1	98387	PASS
365	198	1	100	4.1	14828	PASS
441	198	0.01	100	12.5	45315	PASS
442	442	100	100	100.0	295147	PASS
443	442	15	24	20.3	59971	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/24/2023	BNA_P	<u>BP015272.D</u>
Compound Name	Response	Retention Time
DDT	1124467	20.869
DDD	10846	20.492
DDE	190	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11036	1135503	0.97

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015272.D
 Acq On : 24 May 2023 14:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:06:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

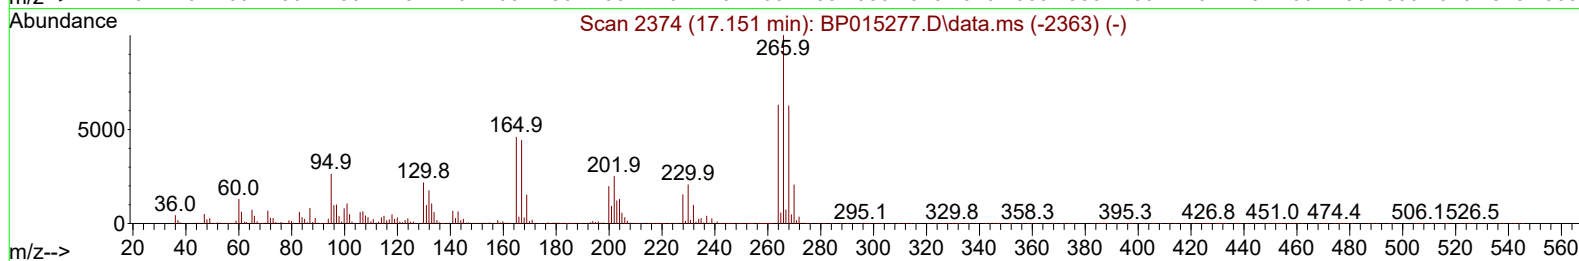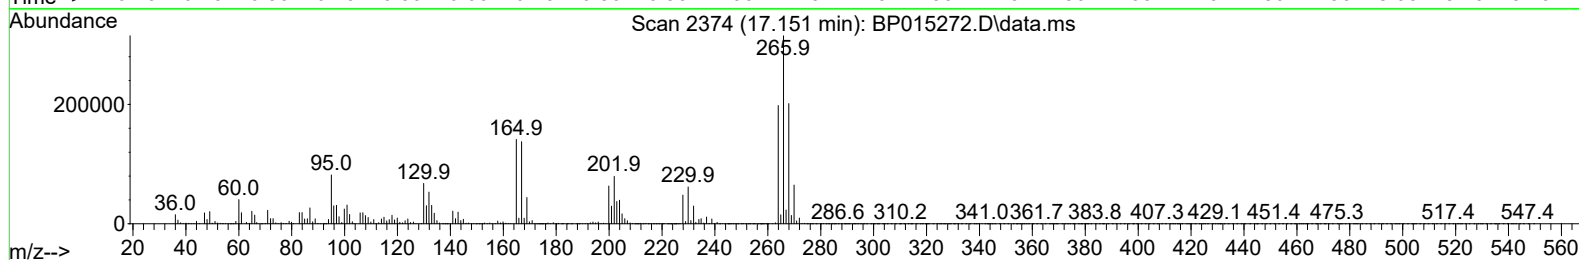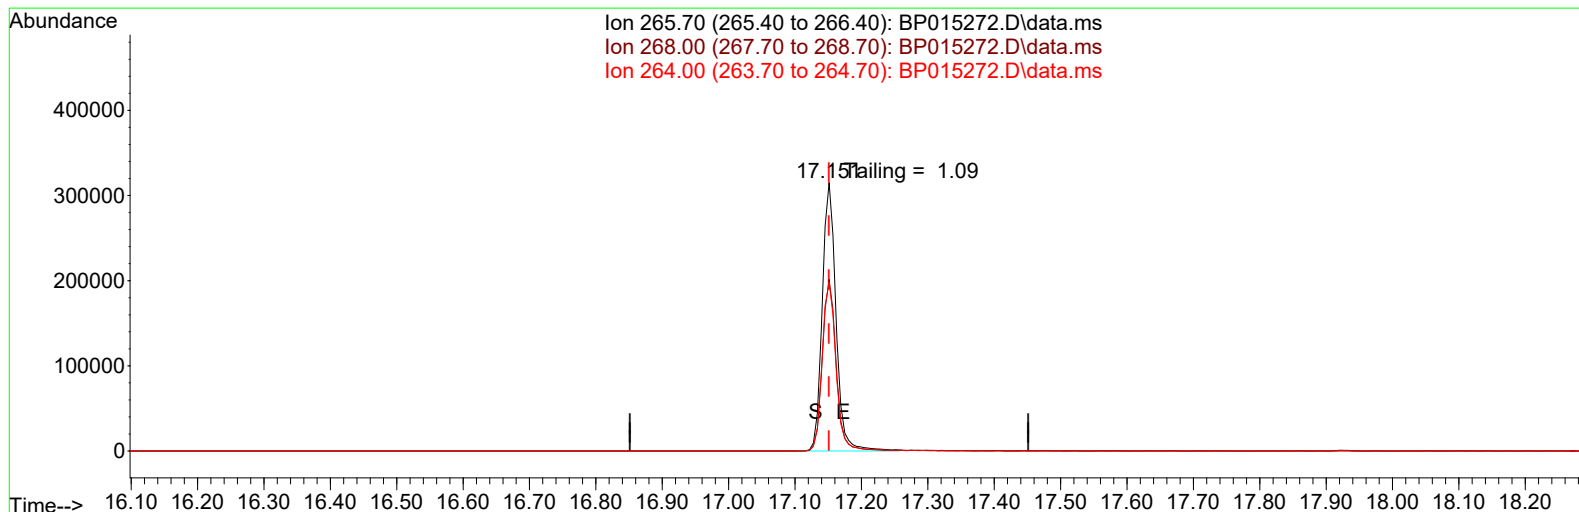

TIC: BP015272.D\data.ms

(70) Pentachlorophenol (C)

17.151min (+ 0.000) 847485.04 ng




response 456440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.89
264.00	63.00	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052423\
 Data File : BP015272.D
 Acq On : 24 May 2023 14:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:06:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 25 01:41:43 2023
 Response via : Initial Calibration

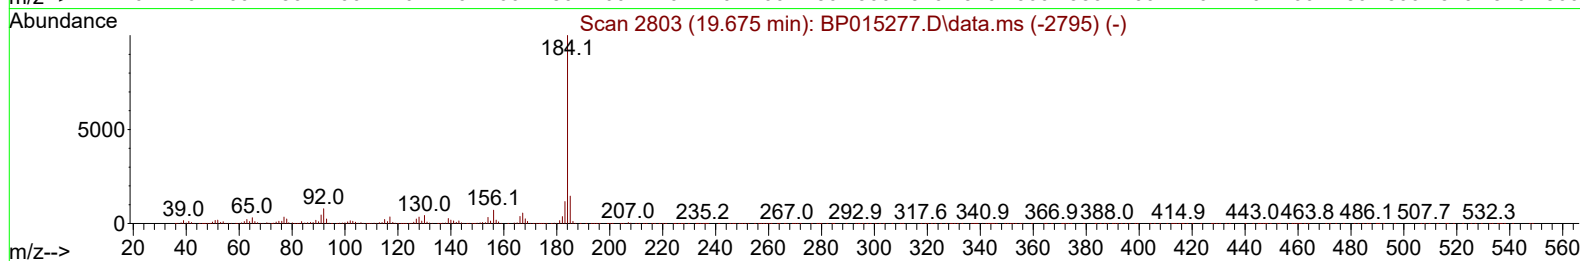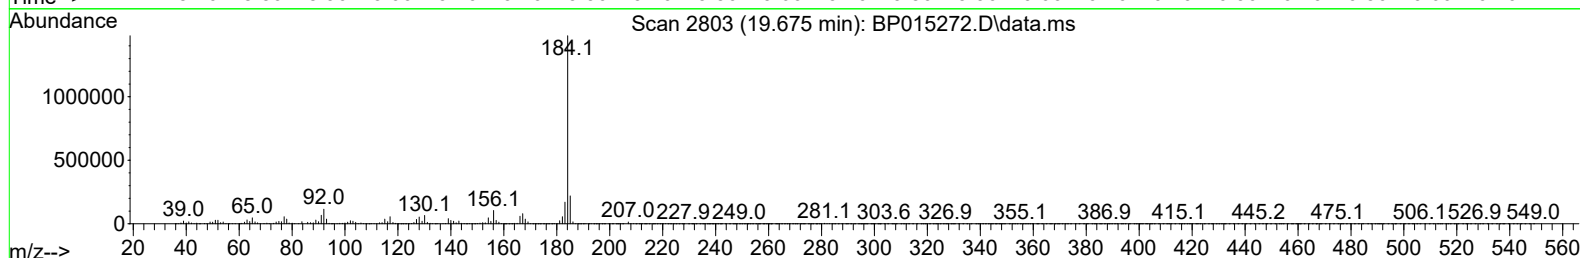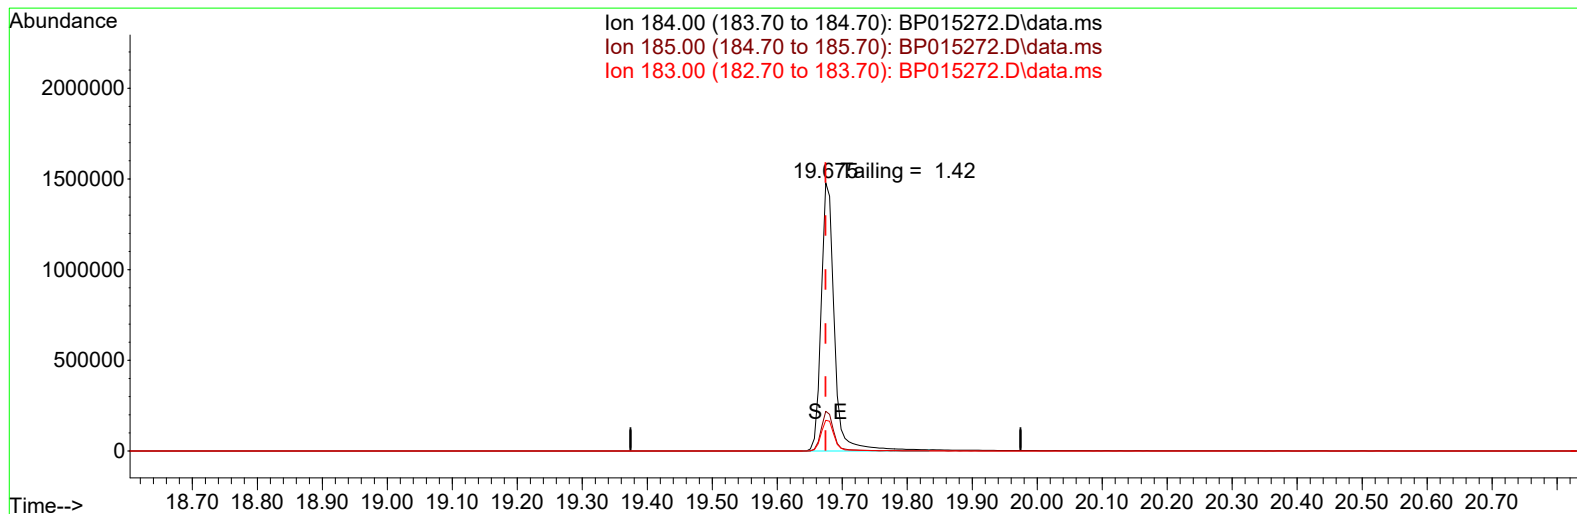

TIC: BP015272.D\data.ms

(77) Benzidine

19.675min (+ 0.000) 1094623.71 ng

response 2097378

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.79
183.00	11.70	11.46
0.00	0.00	0.00