


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052720\
 Data File : BP002290.D
 Acq On : 27 May 2020 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 11:01:43 2020

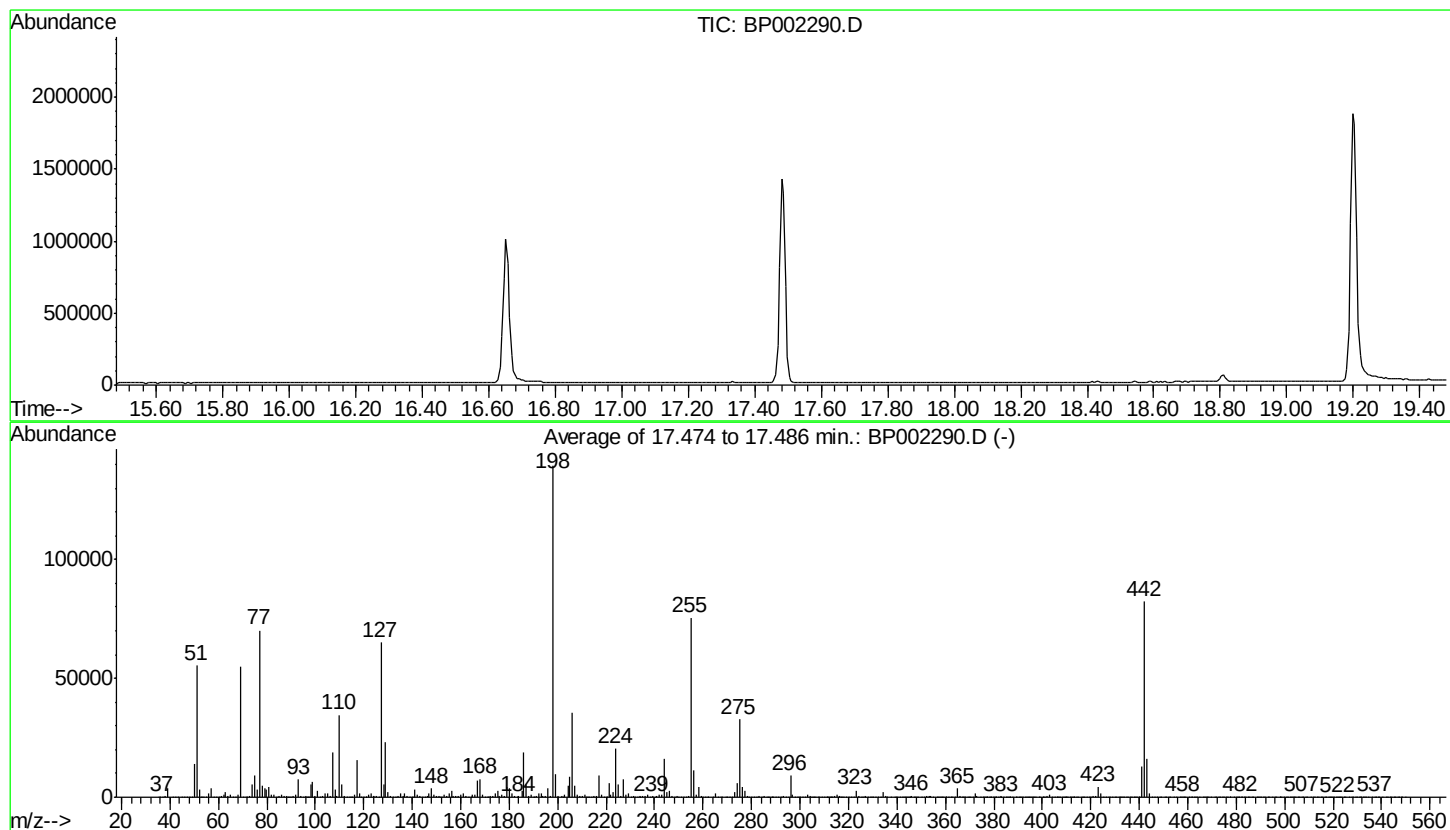

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	55229	PASS
68	69	0.00	2	1.8	1018	PASS
69	198	0.00	100	39.5	55112	PASS
70	69	0.00	2	0.4	237	PASS
127	198	10	80	46.7	65100	PASS
197	198	0.00	2	0.4	537	PASS
198	198	100	100	100.0	139429	PASS
199	198	5	9	7.1	9940	PASS
275	198	10	60	23.5	32743	PASS
365	198	1	100	2.7	3709	PASS
441	198	0.01	100	9.3	12955	PASS
442	198	50	100	58.9	82159	PASS
443	442	15	24	19.8	16251	PASS