
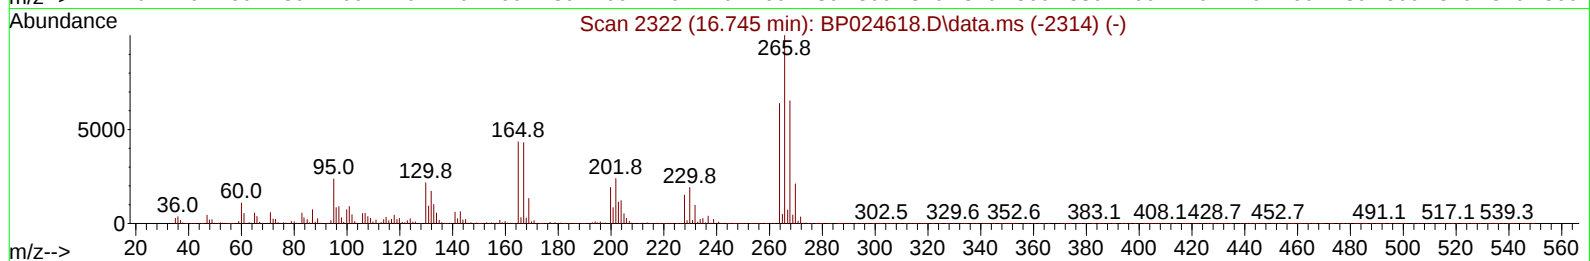
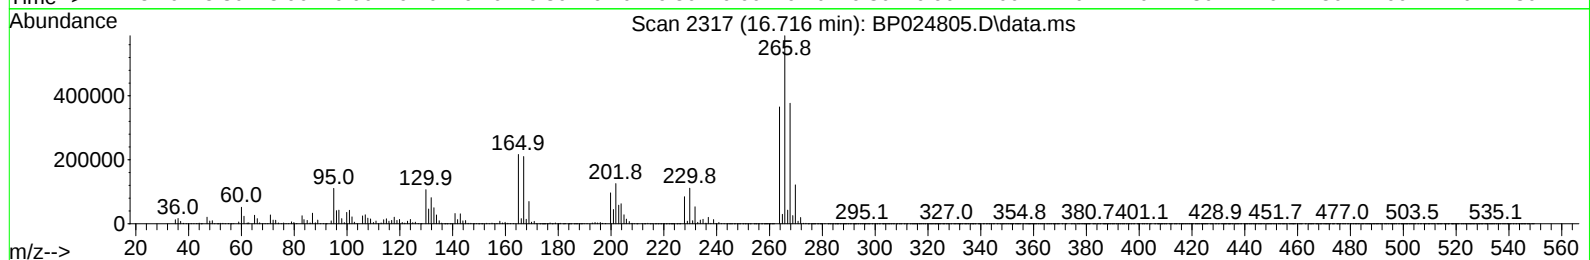


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052725\
Data File : BP024805.D
Acq On : 27 May 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 10:52:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

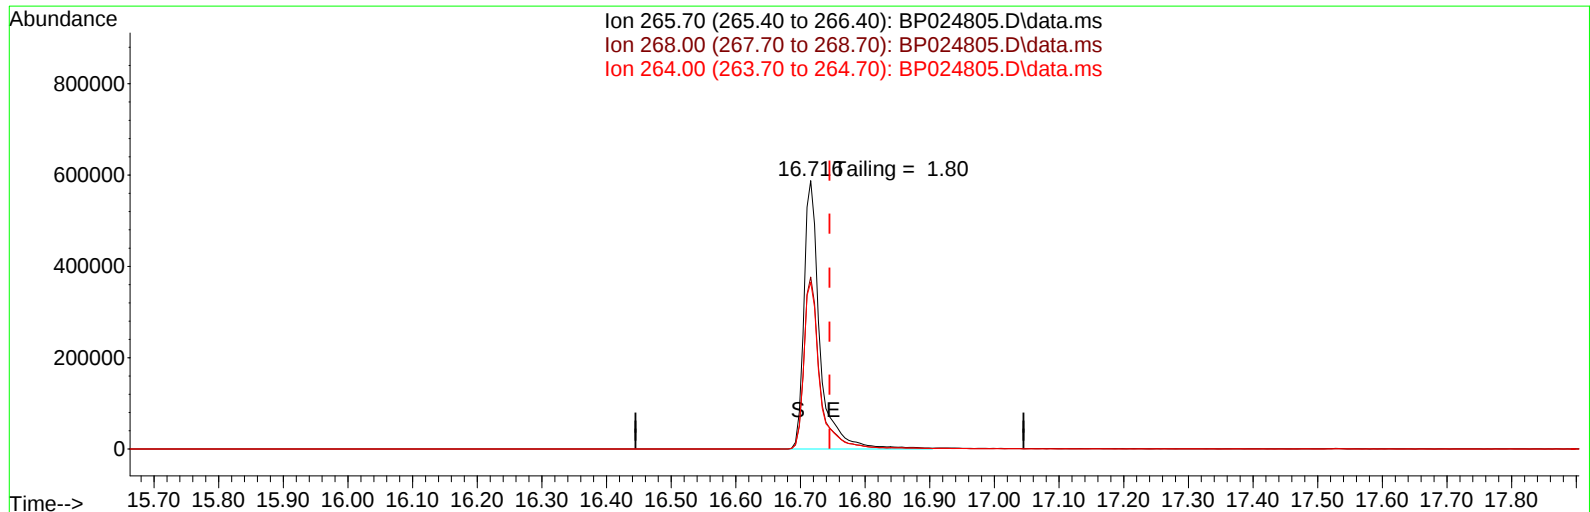

TIC: BP024805.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.029) 497847.44 ng

response 1008451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.10
264.00	63.90	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052725\
Data File : BP024805.D
Acq On : 27 May 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 10:52:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

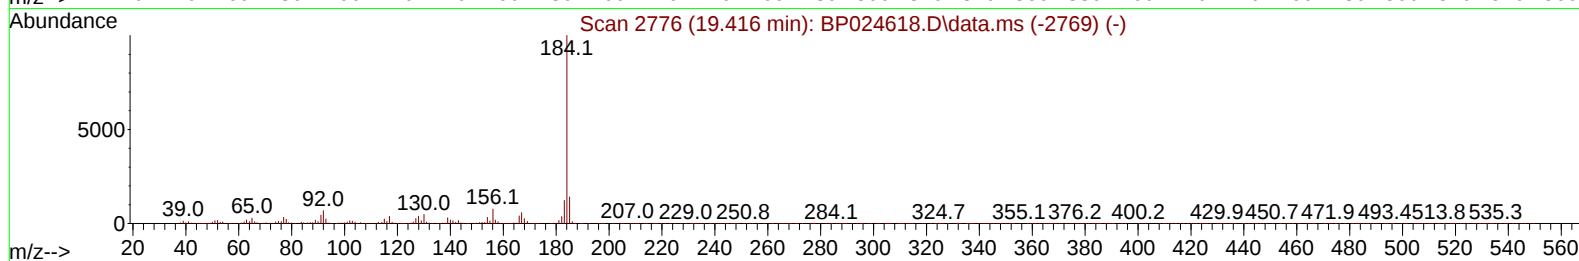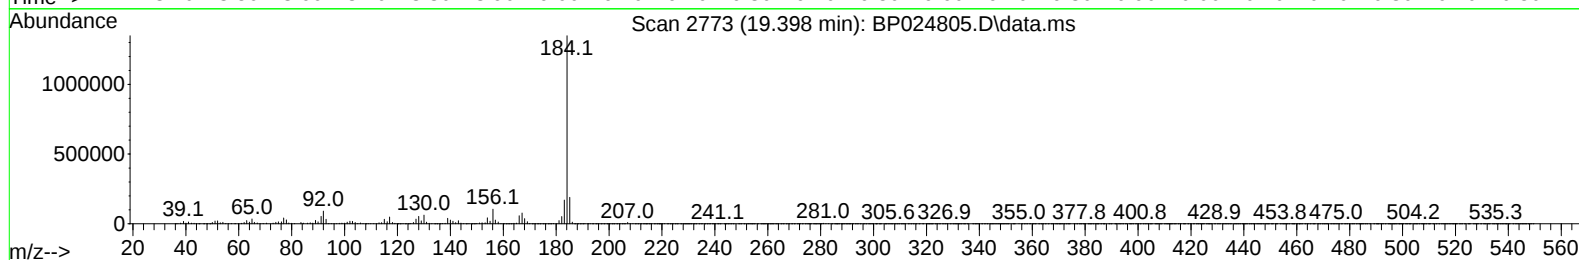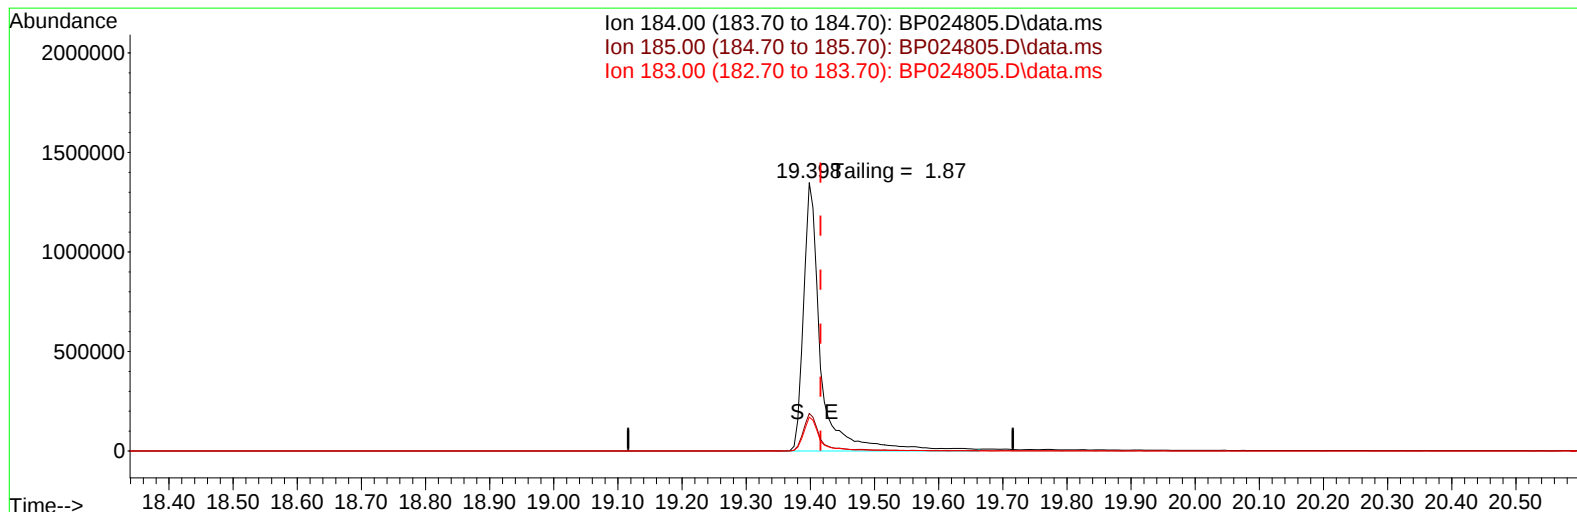

TIC: BP024805.D\data.ms

(77) Benzidine

19.398min (-0.018) 36155.31 ng

response **2498245**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	12.30	12.64
0.00	0.00	0.00