
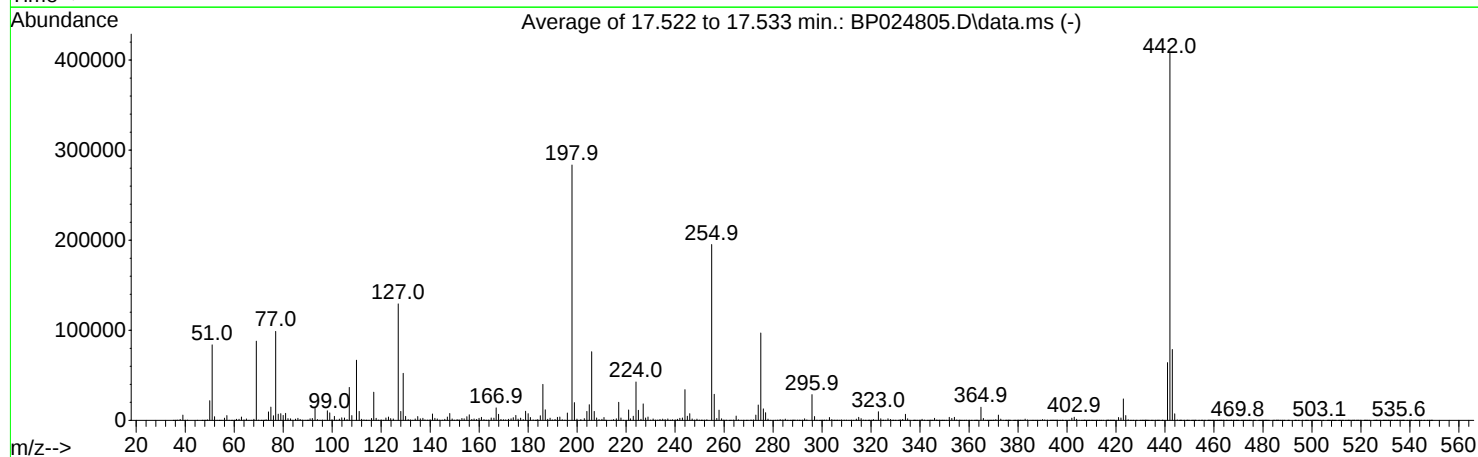


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052725\
Data File : BP024805.D
Acq On : 27 May 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 28 14:16:13 2025

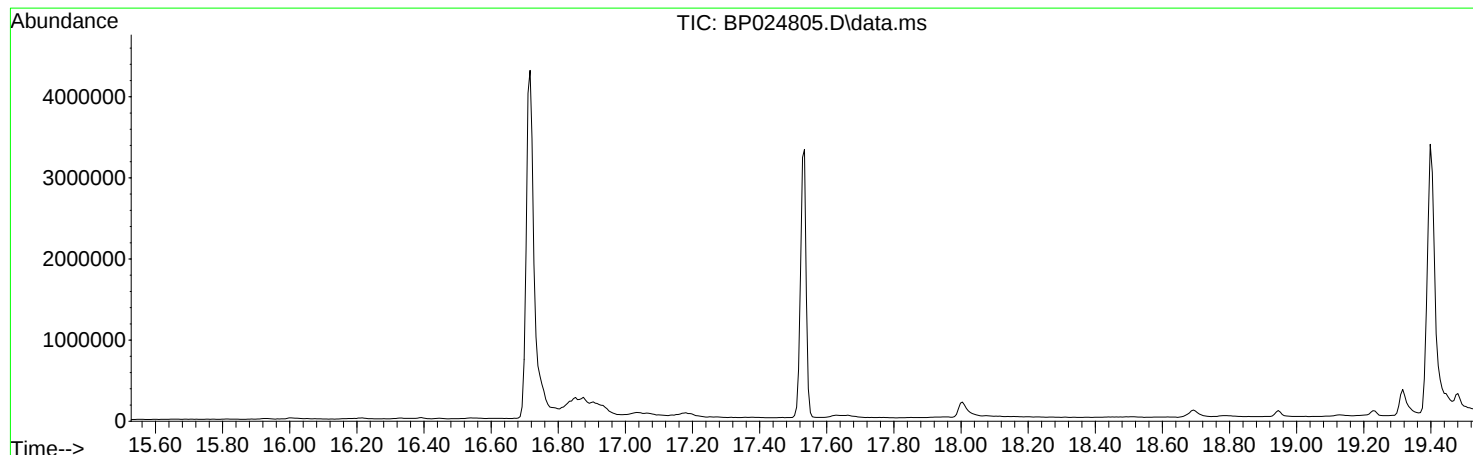




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	83800	PASS
68	69	0.00	2	1.4	1192	PASS
69	198	0.00	100	31.0	87864	PASS
70	69	0.00	2	0.5	431	PASS
127	198	10	80	45.6	129259	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	283499	PASS
199	198	5	9	7.0	19711	PASS
275	198	10	60	34.2	97080	PASS
365	198	1	100	5.1	14581	PASS
441	198	0.01	100	22.6	64120	PASS
442	442	100	100	100.0	408394	PASS
443	442	15	24	19.3	78750	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052725\
Data File : BP024805.D
Acq On : 27 May 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 27 10:52:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

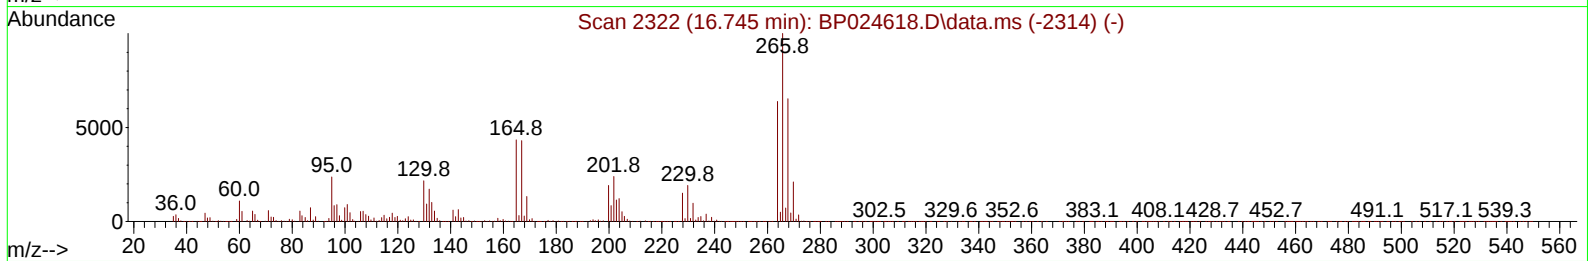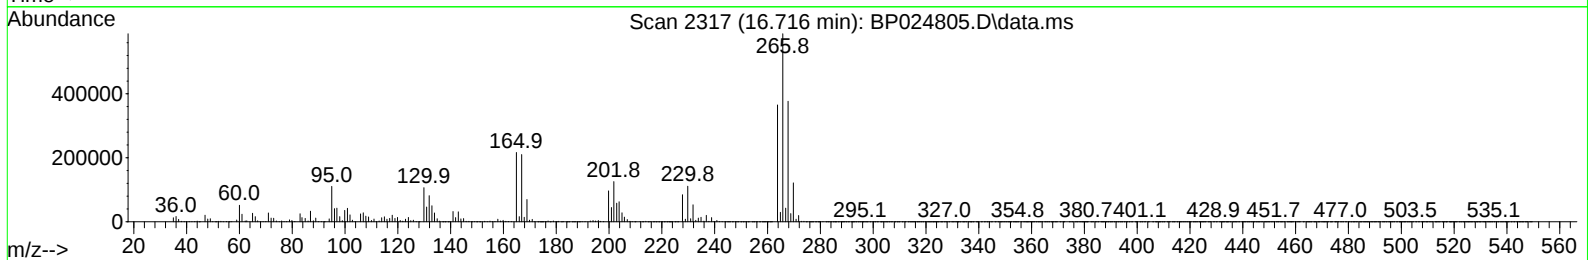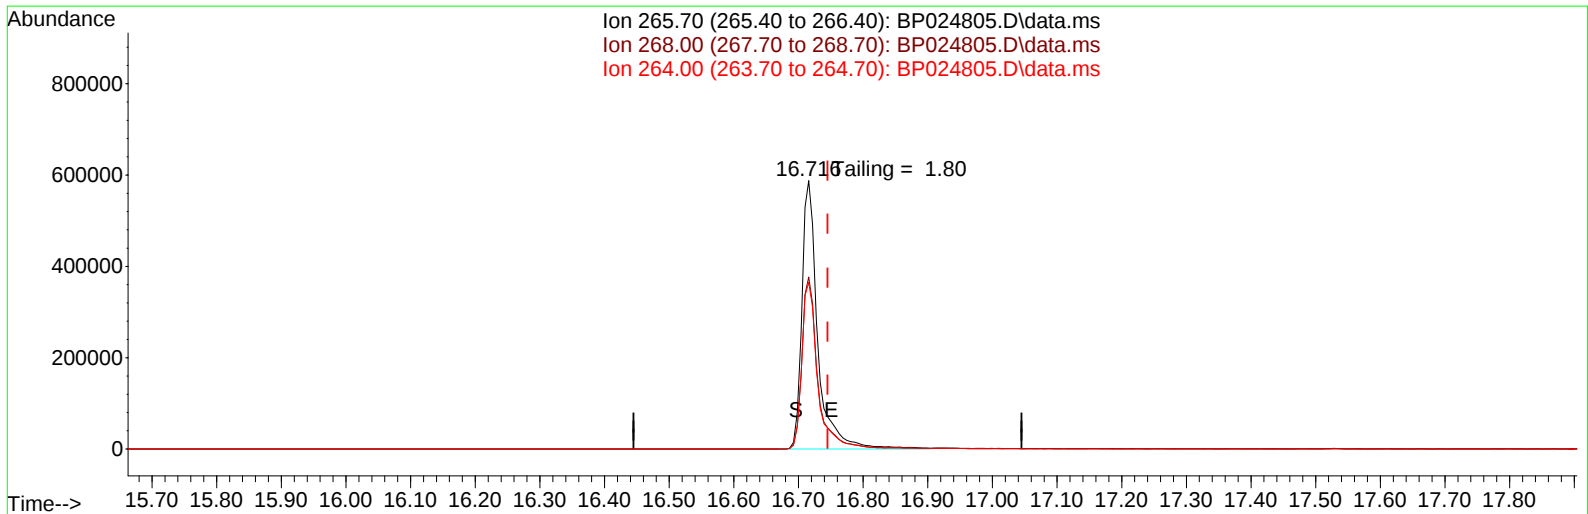

TIC: BP024805.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.029) 497847.44 ng




response 1008451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.10
264.00	63.90	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052725\
Data File : BP024805.D
Acq On : 27 May 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 27 10:52:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

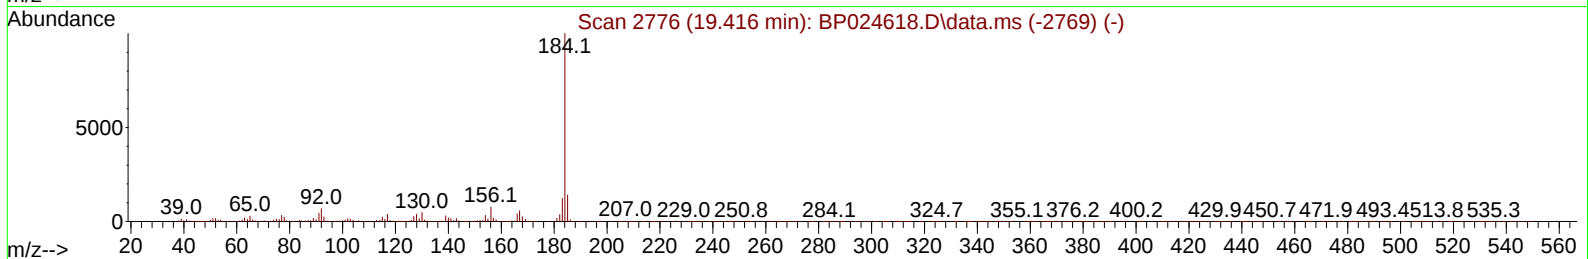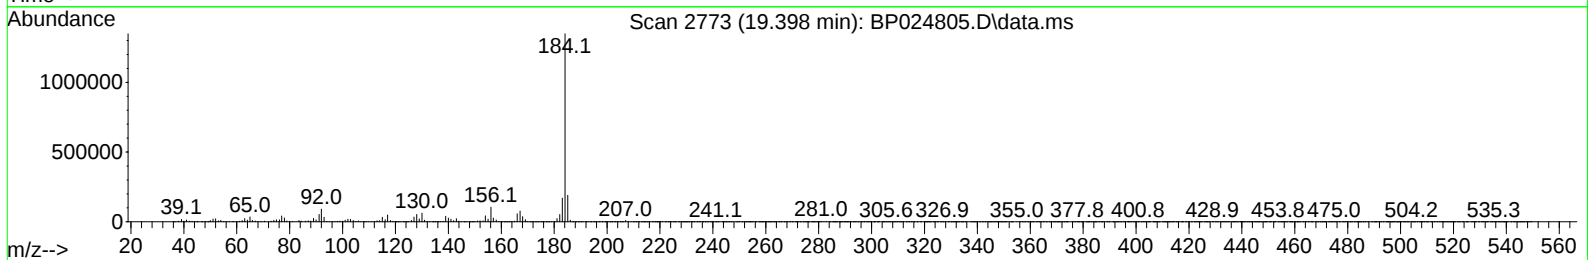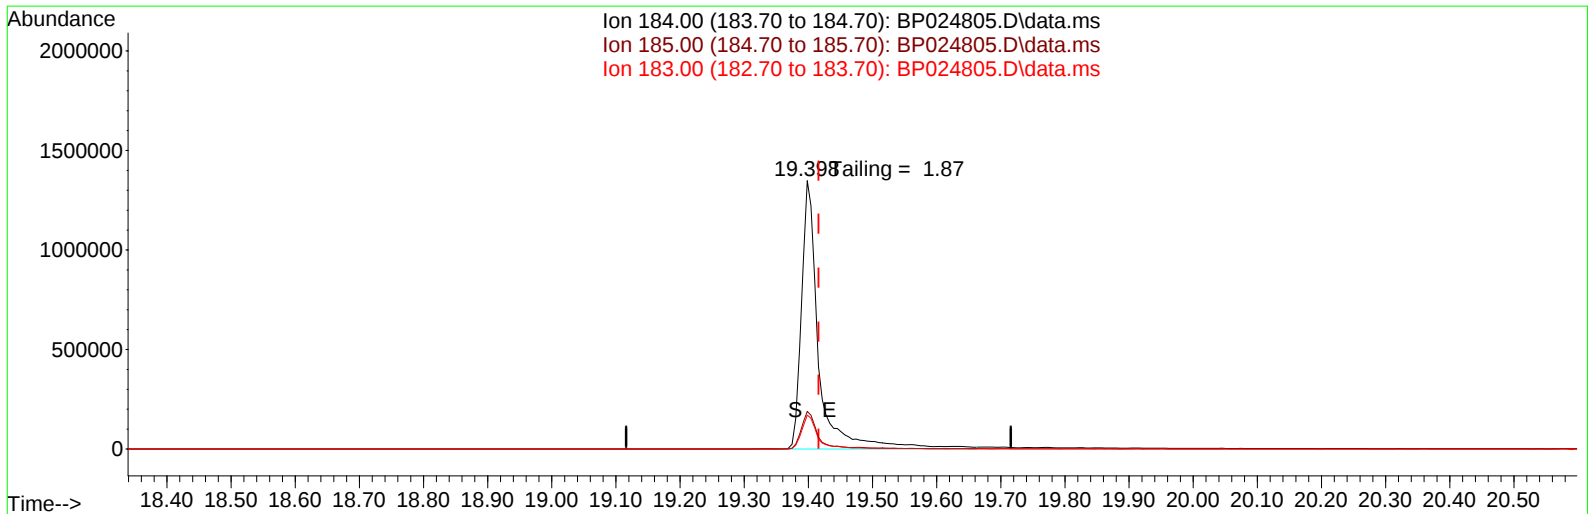

TIC: BP024805.D\data.ms

(77) Benzidine

19.398min (-0.018) 36155.31 ng

response 2498245

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.04
183.00	12.30	12.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/27/2025	BNA_P	<u>BP024805.D</u>
Compound Name	Response	Retention Time
DDT	1037349	20.68
DDD	38120	20.222
DDE	2359	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40479	1077828	3.76

Instrument :
BNA_P
ClientSampleId :
DFTPP