
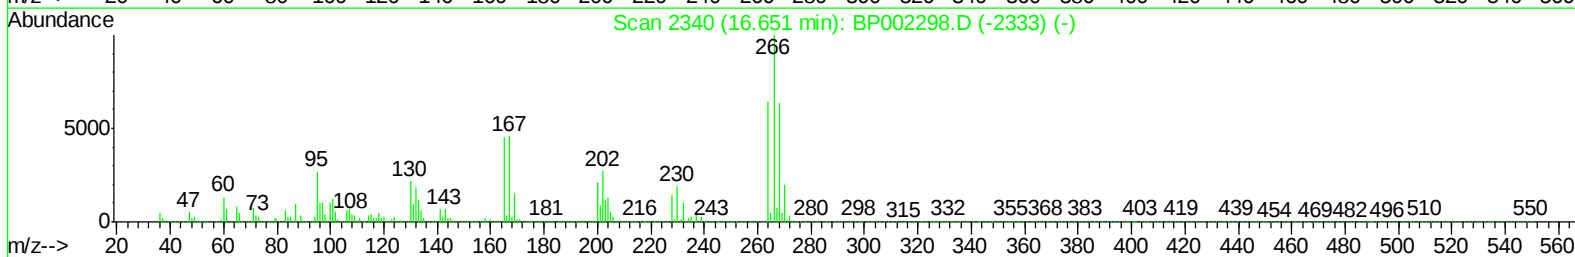
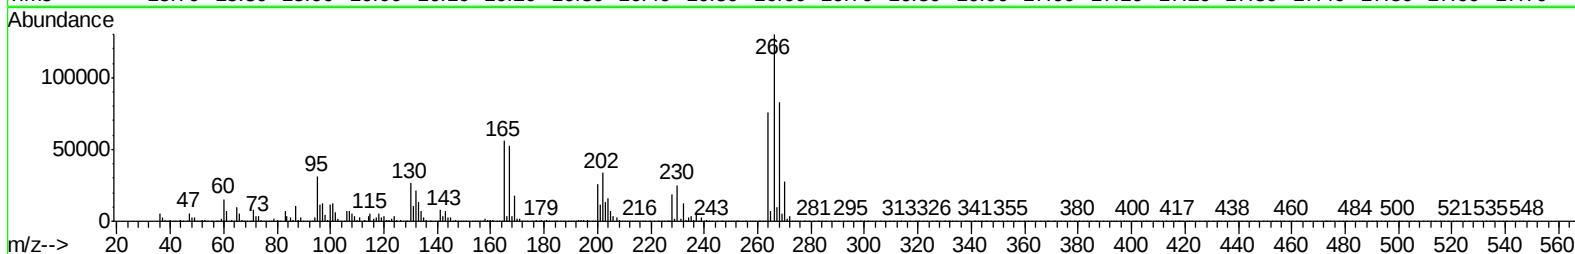


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP052820\
 Data File : BP002300.D
 Acq On : 28 May 2020 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 03:20:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 28 11:01:43 2020
 Response via : Initial Calibration

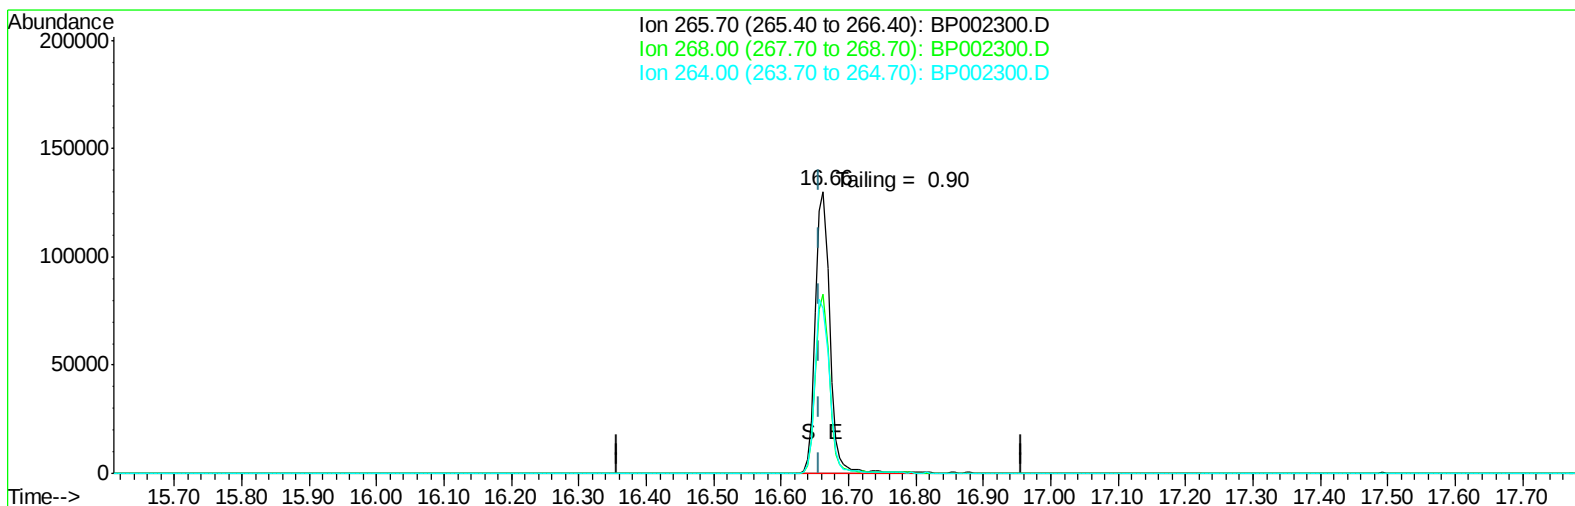

TIC: BP002300.D

(70) Pentachlorophenol (C)




16.663min (+0.006) 46542.51ng

response 189847

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.48
264.00	60.40	58.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP052820\
 Data File : BP002300.D
 Acq On : 28 May 2020 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 03:20:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 28 11:01:43 2020
 Response via : Initial Calibration

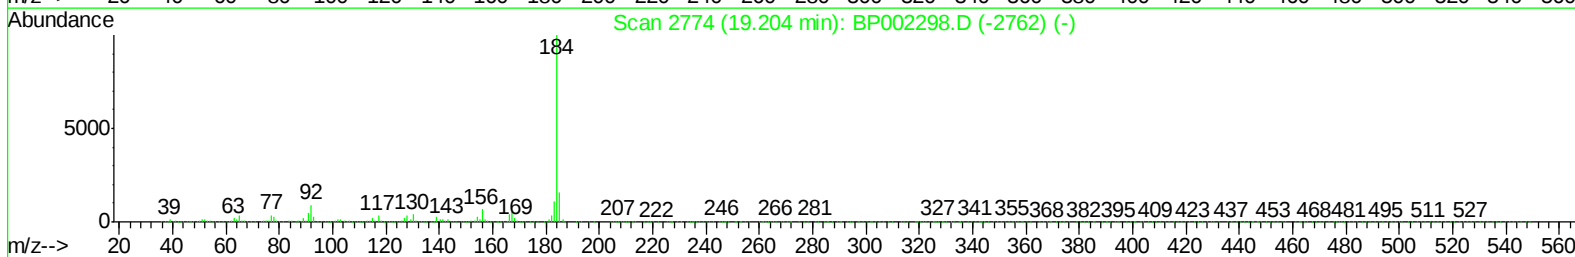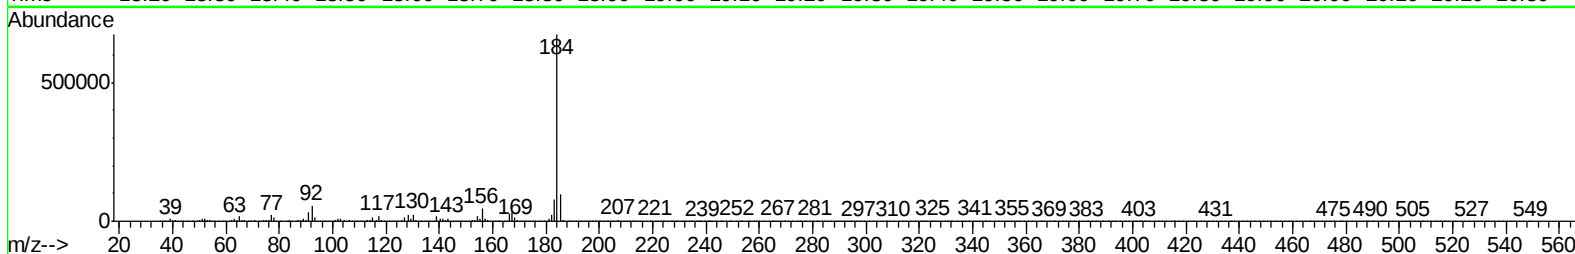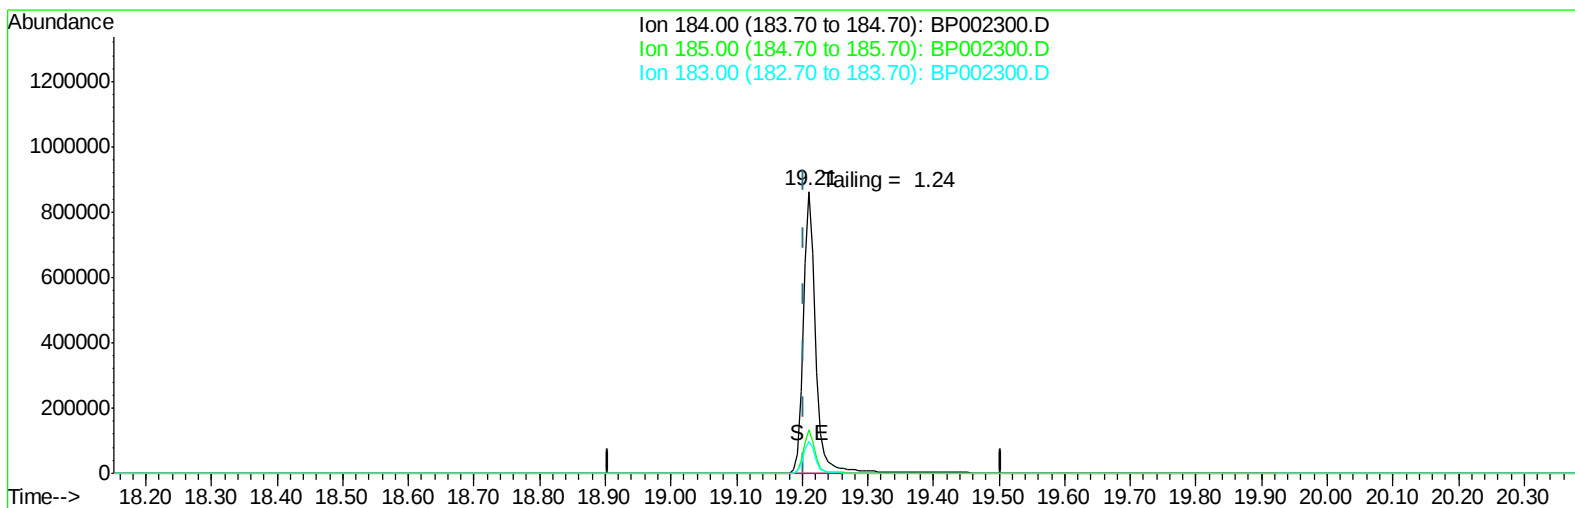

TIC: BP002300.D

(77) Benzidine

19.210min (+0.006) 1519072.76ng

response 1141402

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.31
183.00	11.40	11.17
0.00	0.00	0.00