
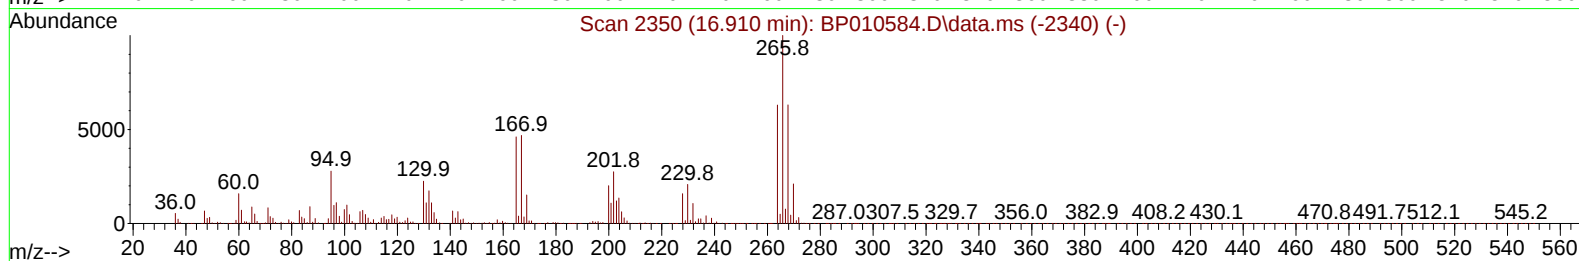
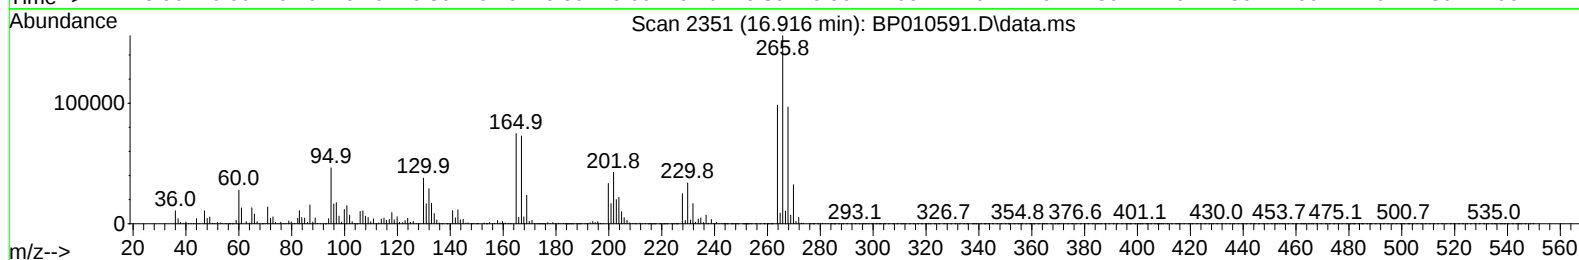


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010591.D
 Acq On : 28 May 2022 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 04:44:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

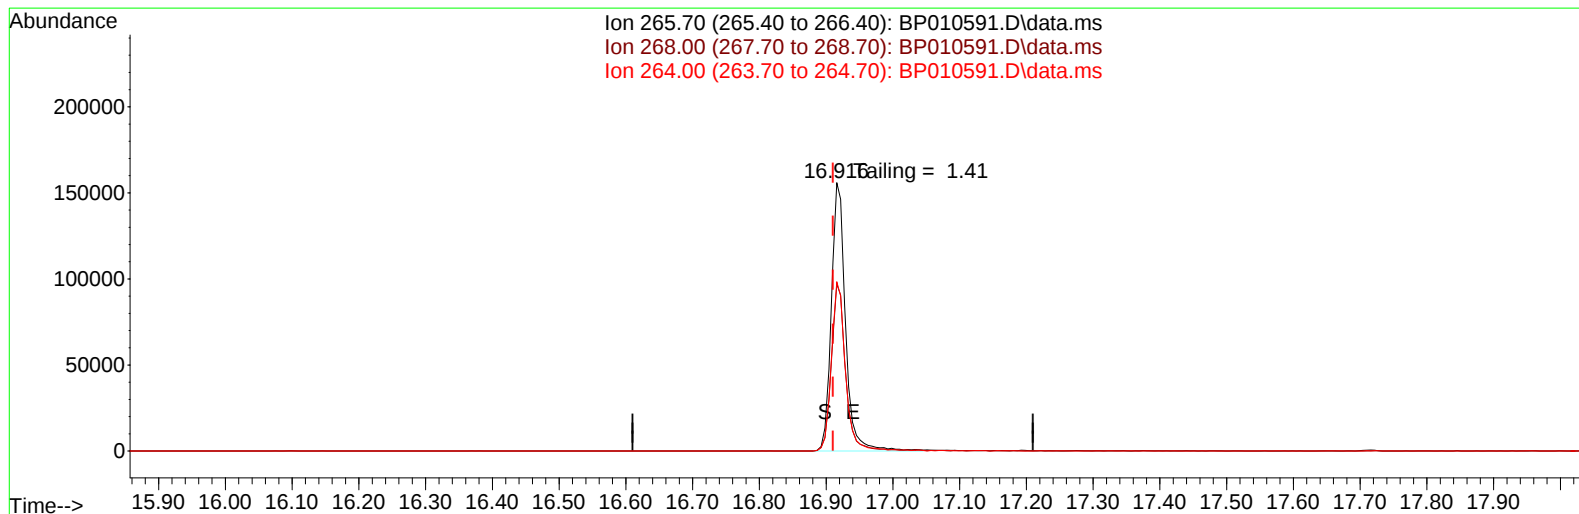

TIC: BP010591.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.006) 208856.10 ng

response 230504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.15
264.00	63.00	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010591.D
 Acq On : 28 May 2022 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 04:44:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

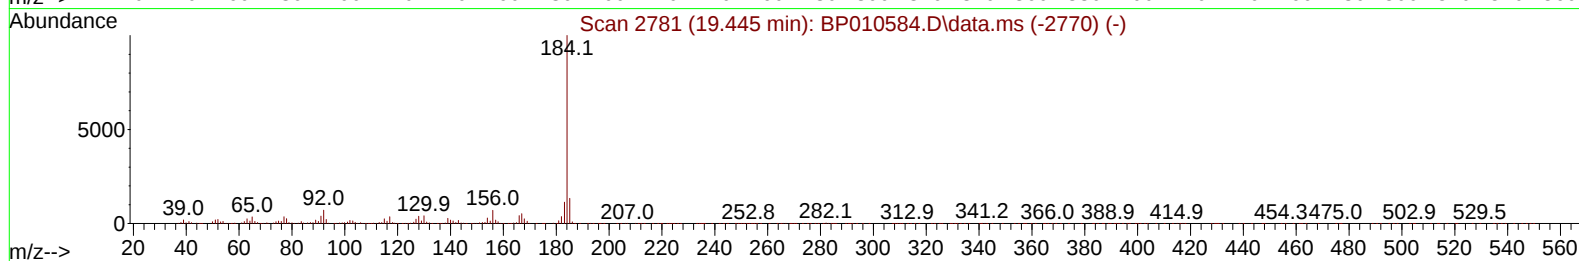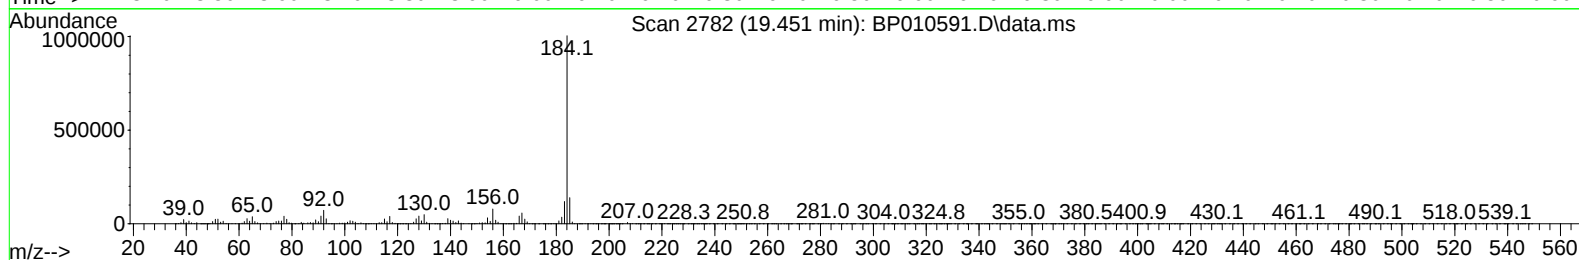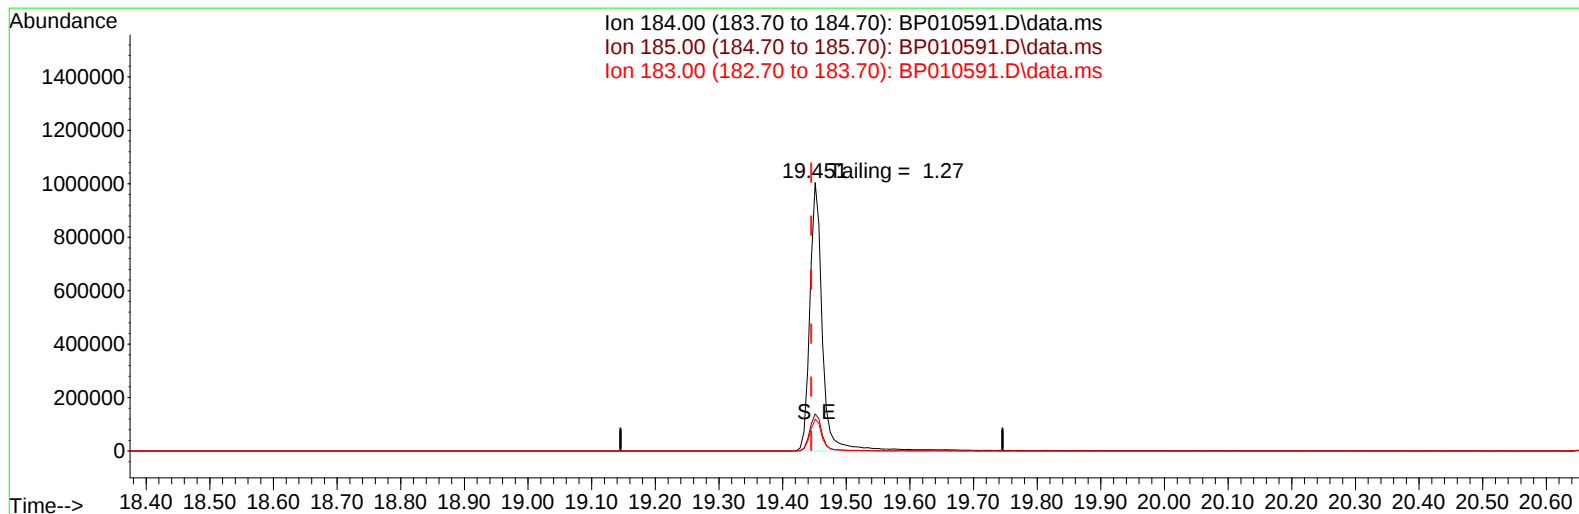

TIC: BP010591.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 20319.56 ng

response 1386046

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.85
183.00	11.30	11.85
0.00	0.00	0.00