

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010589.D
Acq On : 28 May 2022 01:47
Operator : CG/JU
Sample : PB145173BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145173BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	395	401	415	rBV	2945186	4359303	64.37%	12.406%
2	7.040	664	672	690	rBV	2859782	4516226	66.68%	12.852%
3	7.869	806	813	826	rBV	490987	792592	11.70%	2.256%
4	9.028	1001	1010	1033	rBV	1702067	2977762	43.97%	8.474%
5	10.669	1280	1289	1312	rBV	561546	1055875	15.59%	3.005%
6	13.128	1699	1707	1725	rBV	3917379	5941070	87.72%	16.907%
7	14.504	1933	1941	1955	rBV	857256	1335518	19.72%	3.801%
8	15.992	2187	2194	2215	rBV	2742537	3933295	58.08%	11.193%
9	17.257	2402	2409	2423	rBV	885051	1370033	20.23%	3.899%
10	19.810	2838	2843	2856	rBV	5636772	6772525	100.00%	19.273%
11	21.339	3098	3103	3115	rBV	857197	1177334	17.38%	3.350%
12	23.751	3507	3513	3523	rVB	430227	907711	13.40%	2.583%




Sum of corrected areas: 35139244

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010589.D
Acq On : 28 May 2022 01:47
Operator : CG/JU
Sample : PB145173BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145173BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

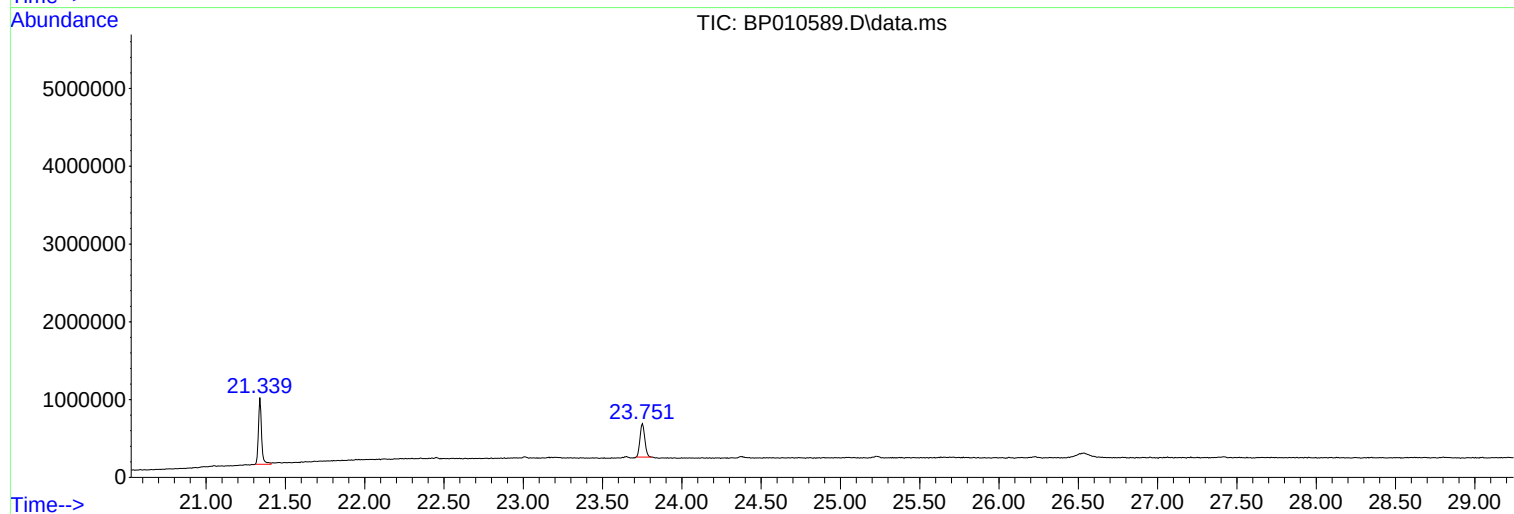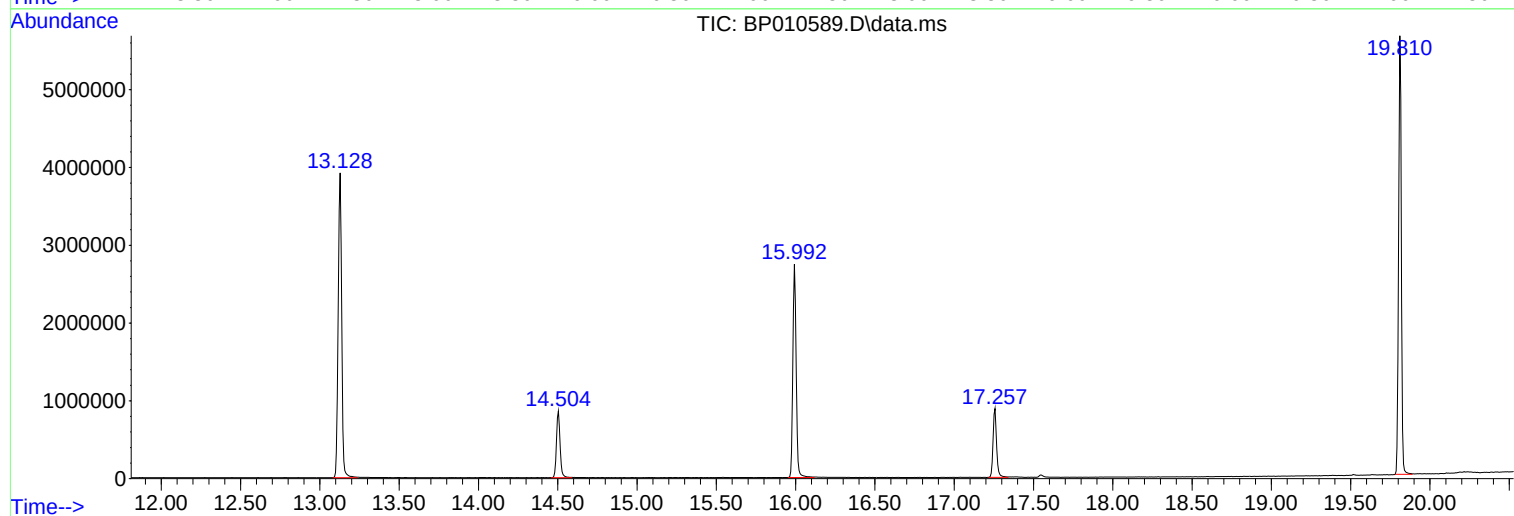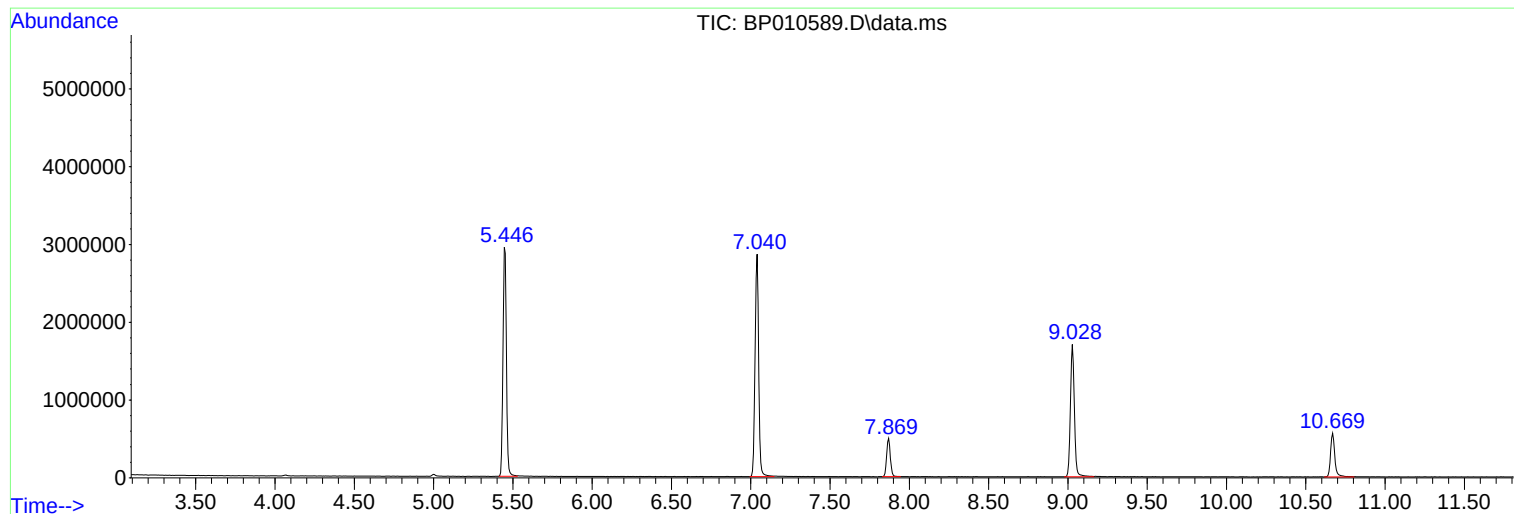

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010589.D
Acq On : 28 May 2022 01:47
Operator : CG/JU
Sample : PB145173BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145173BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010589.D
Acq On : 28 May 2022 01:47
Operator : CG/JU
Sample : PB145173BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145173BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------