

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010603.D
 Acq On : 28 May 2022 16:51
 Operator : CG/JU
 Sample : N2931-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P016-SS002-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010603.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	394	401	415	rBV	2114255	3199670	24.43%	6.395%
2	7.034	663	671	687	rBV	2090600	3520581	26.88%	7.037%
3	7.863	805	812	820	rBV	518865	852758	6.51%	1.704%
4	9.022	1001	1009	1026	rBV	1274667	2269219	17.33%	4.536%
5	10.663	1279	1288	1301	rBV	666002	1199612	9.16%	2.398%
6	13.122	1699	1706	1725	rBV	3015730	4513953	34.47%	9.022%
7	14.498	1933	1940	1954	rBV	1049022	1554865	11.87%	3.108%
8	15.992	2187	2194	2212	rBV	2526574	3781627	28.88%	7.558%
9	17.251	2399	2408	2414	rBV	1271792	1879739	14.35%	3.757%
10	17.928	2519	2523	2528	rBV	169571	192706	1.47%	0.385%
11	18.145	2555	2560	2569	rBV	350173	581988	4.44%	1.163%
12	19.375	2765	2769	2778	rBV2	164992	264626	2.02%	0.529%
13	19.810	2838	2843	2854	rBV	5765145	6840467	52.23%	13.672%
14	21.051	3049	3054	3061	rBV	495803	746109	5.70%	1.491%
15	21.245	3084	3087	3094	rBV	432922	486631	3.72%	0.973%
16	21.339	3097	3103	3108	rBV	1705353	2321634	17.73%	4.640%
17	21.457	3117	3123	3141	rBV	8954668	13095606	100.00%	26.175%
18	21.774	3175	3177	3184	rVB	97033	131921	1.01%	0.264%
19	23.010	3383	3387	3392	rBV2	156204	237827	1.82%	0.475%
20	23.745	3506	3512	3526	rVB2	1121015	2360044	18.02%	4.717%




Sum of corrected areas: 50031583

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010603.D
Acq On : 28 May 2022 16:51
Operator : CG/JU
Sample : N2931-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

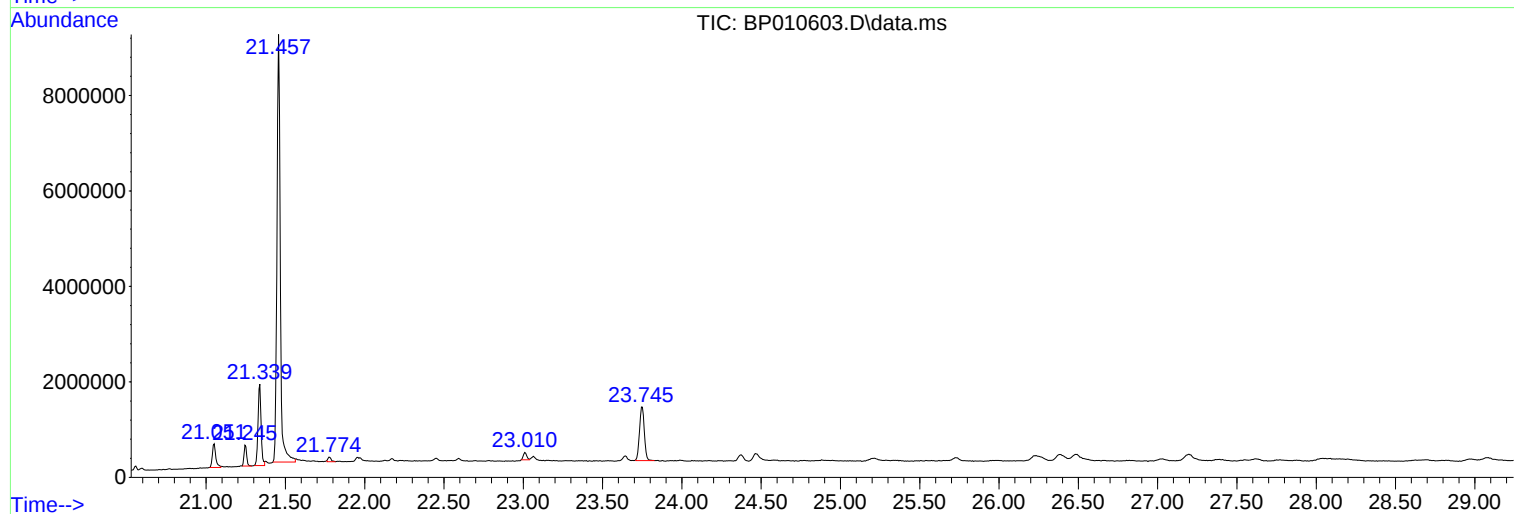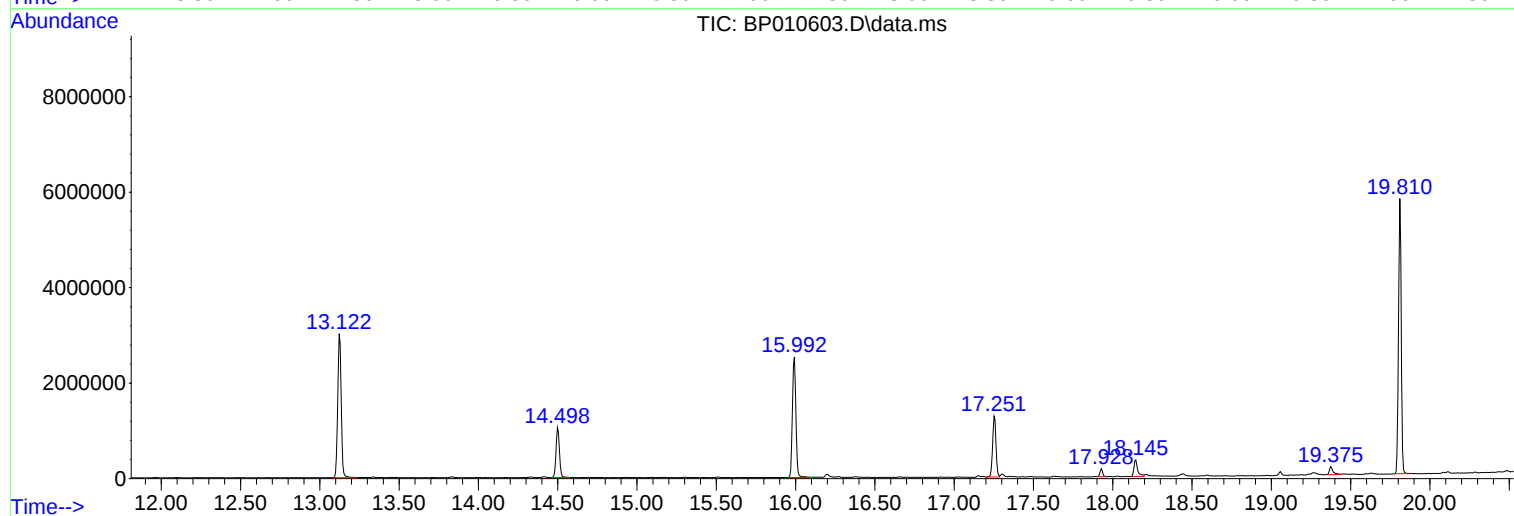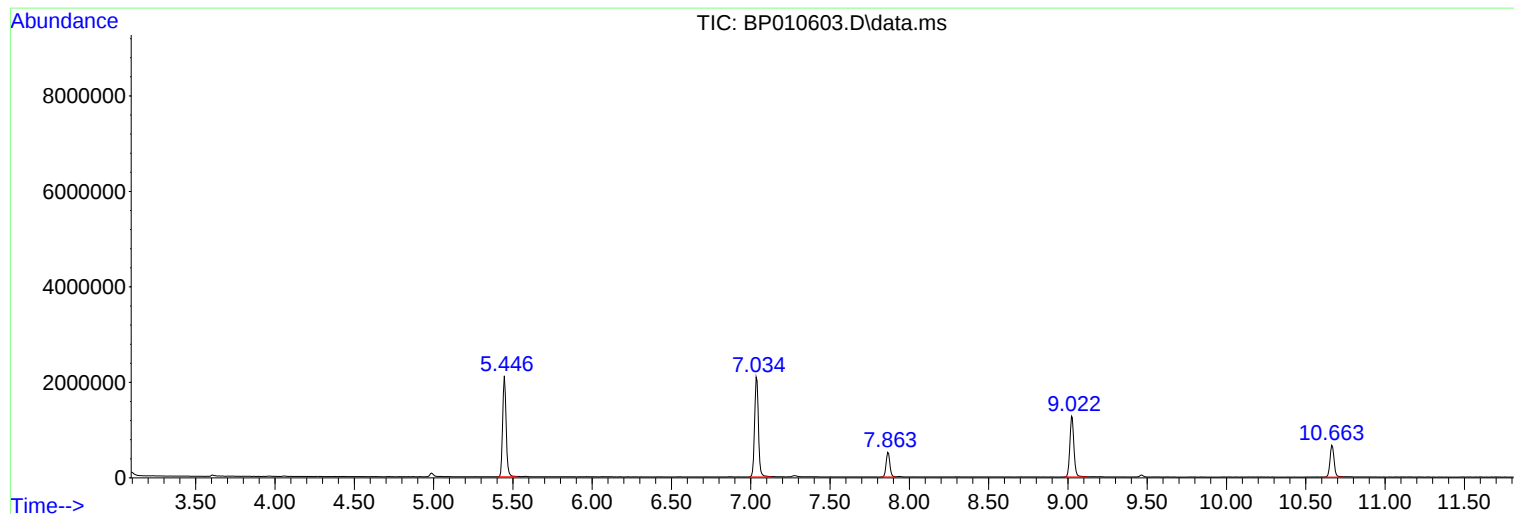

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010603.D
Acq On : 28 May 2022 16:51
Operator : CG/JU
Sample : N2931-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010603.D
Acq On : 28 May 2022 16:51
Operator : CG/JU
Sample : N2931-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------