

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010607.D
 Acq On : 28 May 2022 19:07
 Operator : CG/JU
 Sample : N2933-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P023-SS002-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	393	402	418	rBV	2912977	4538359	38.24%	5.647%
2	7.040	662	672	688	rBV	3005436	5049113	42.55%	6.283%
3	7.863	805	812	820	rBV	610795	1007475	8.49%	1.254%
4	9.028	1002	1010	1026	rBV	1840881	3172764	26.74%	3.948%
5	10.381	1232	1240	1252	rBV	67725	178466	1.50%	0.222%
6	10.663	1280	1288	1300	rBV	858170	1484946	12.51%	1.848%
7	10.863	1315	1322	1336	rBV	127022	265229	2.23%	0.330%
8	12.446	1583	1591	1608	rBV2	44120	167113	1.41%	0.208%
9	13.122	1699	1706	1724	rBV	4342923	6577058	55.42%	8.184%
10	14.504	1934	1941	1947	rBV	1328098	1998877	16.84%	2.487%
11	14.922	2004	2012	2024	rBV2	78904	163498	1.38%	0.203%
12	15.992	2187	2194	2202	rBV	4120385	5820510	49.05%	7.243%
13	16.457	2267	2273	2284	rBV3	155443	283598	2.39%	0.353%
14	16.657	2302	2307	2318	rBV3	73876	132907	1.12%	0.165%
15	17.251	2400	2408	2414	rVV	1666107	2428346	20.46%	3.022%
16	17.304	2414	2417	2421	rVB2	109681	132893	1.12%	0.165%
17	17.639	2468	2474	2485	rBV7	49373	146128	1.23%	0.182%
18	17.928	2519	2523	2532	rVB	194894	233067	1.96%	0.290%
19	18.145	2555	2560	2568	rBV	776541	1146064	9.66%	1.426%
20	19.057	2711	2715	2719	rVB	321028	356321	3.00%	0.443%
21	19.375	2765	2769	2779	rBV	205121	335580	2.83%	0.418%
22	19.816	2838	2844	2851	rBV	7950209	9864890	83.13%	12.276%
23	20.439	2946	2950	2953	rBV	119459	149373	1.26%	0.186%
24	21.045	3048	3053	3066	rBV2	1298895	1964355	16.55%	2.444%
25	21.245	3084	3087	3092	rVB	803481	888451	7.49%	1.106%
26	21.339	3098	3103	3113	rBV	1945405	2589913	21.82%	3.223%
27	21.457	3117	3123	3138	rBV	7915288	11867093	100.00%	14.767%
28	21.969	3205	3210	3224	rVB2	446968	809104	6.82%	1.007%
29	22.121	3231	3236	3242	rBV	1313113	1877464	15.82%	2.336%
30	23.010	3382	3387	3392	rBV	1608355	2481038	20.91%	3.087%
31	23.063	3392	3396	3403	rVB	414497	758951	6.40%	0.944%
32	23.639	3490	3494	3500	rVB2	305738	555137	4.68%	0.691%
33	23.751	3507	3513	3520	rVB2	994662	2108156	17.76%	2.623%
34	24.374	3613	3619	3627	rVB	1063599	2264447	19.08%	2.818%
35	24.468	3628	3635	3652	rBV	1292000	3414901	28.78%	4.249%
36	26.392	3955	3962	3971	rBV2	518628	1486956	12.53%	1.850%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010607.D
Acq On : 28 May 2022 19:07
Operator : CG/JU
Sample : N2933-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P023-SS002-0006-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	27.204	4092	4100	4111	rVB5	473310	1663630	14.02%	2.070%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 80362171

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010607.D
Acq On : 28 May 2022 19:07
Operator : CG/JU
Sample : N2933-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P023-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

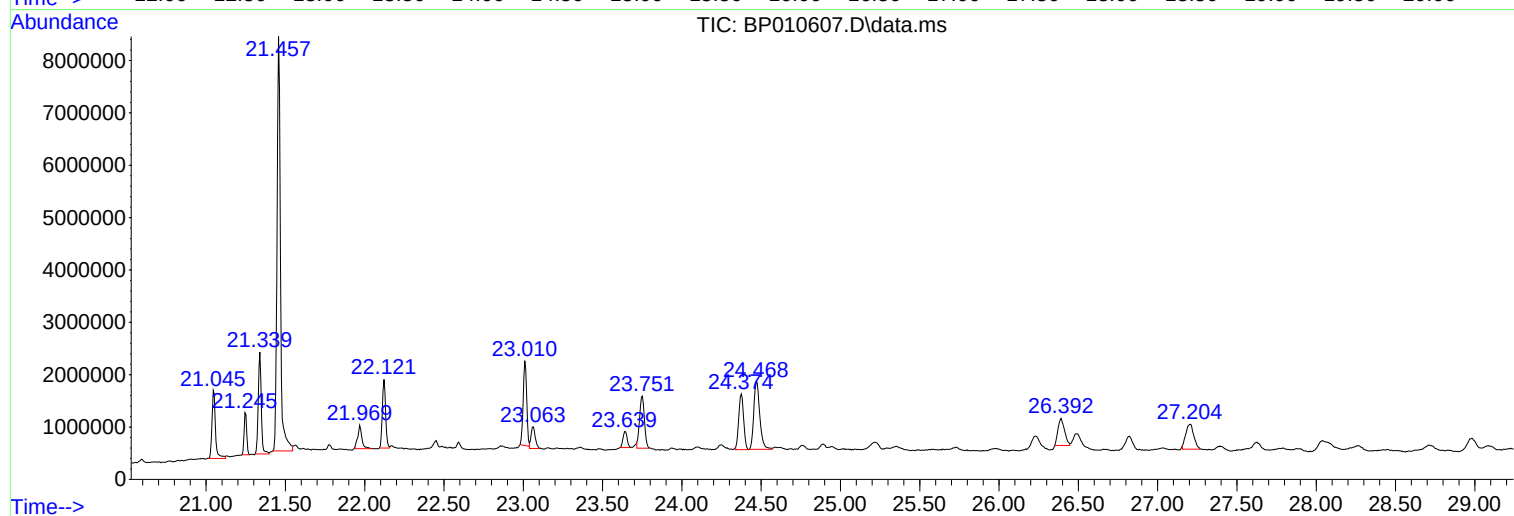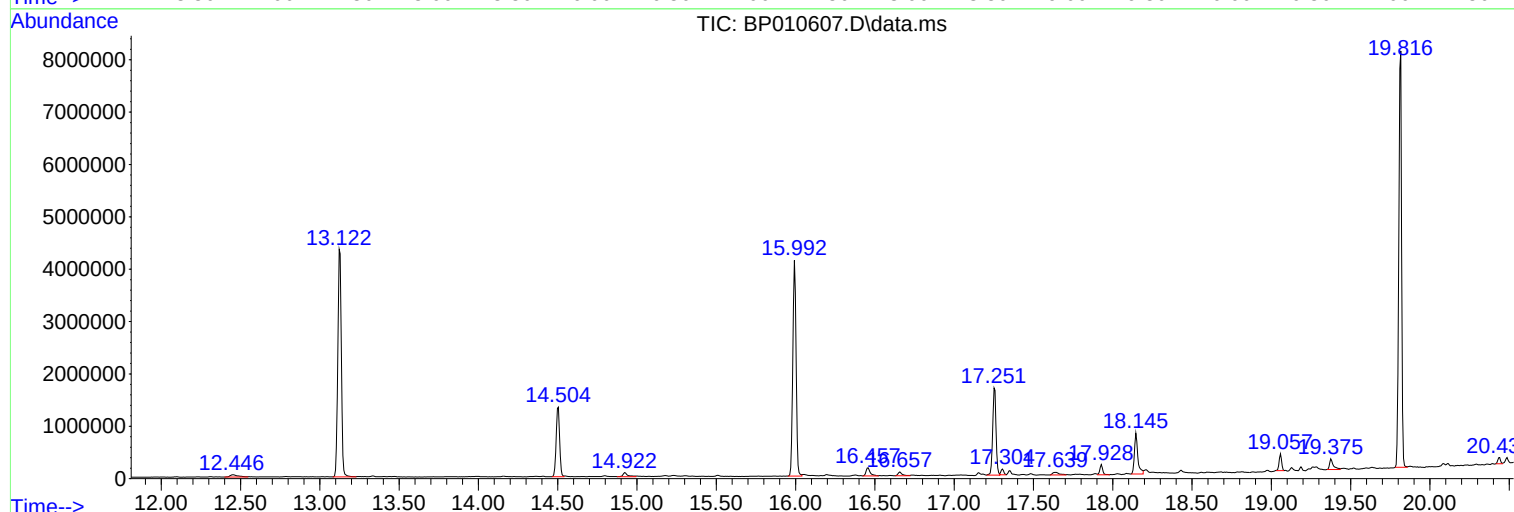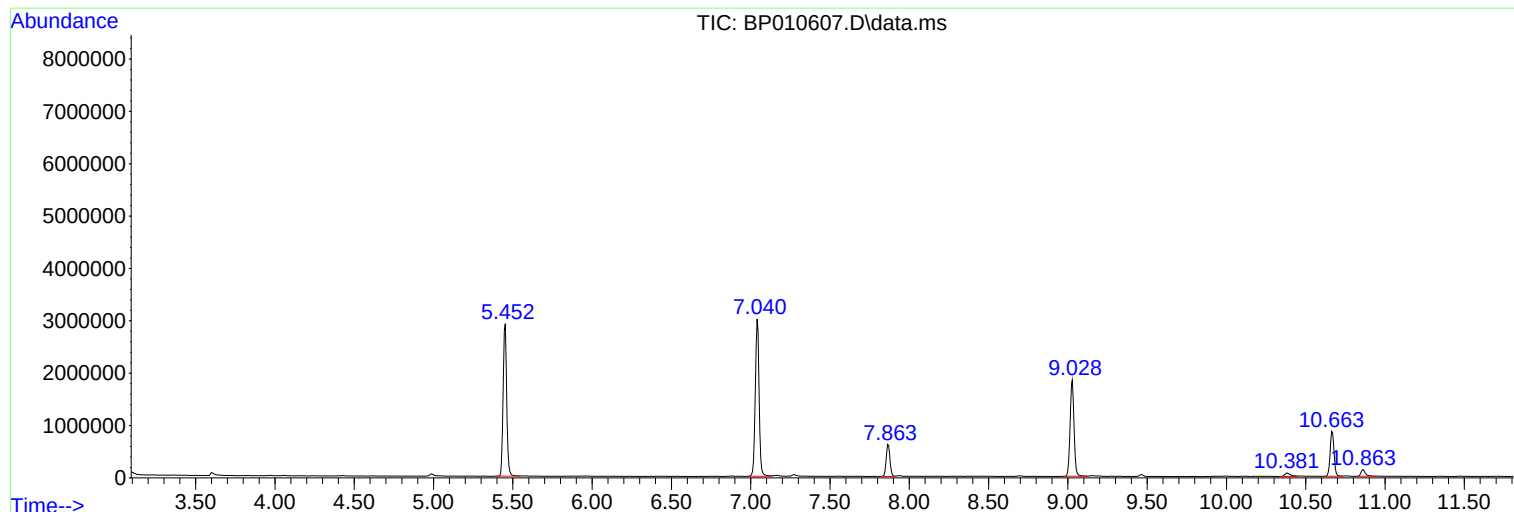

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010607.D
Acq On : 28 May 2022 19:07
Operator : CG/JU
Sample : N2933-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P023-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010607.D
Acq On : 28 May 2022 19:07
Operator : CG/JU
Sample : N2933-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P023-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------