
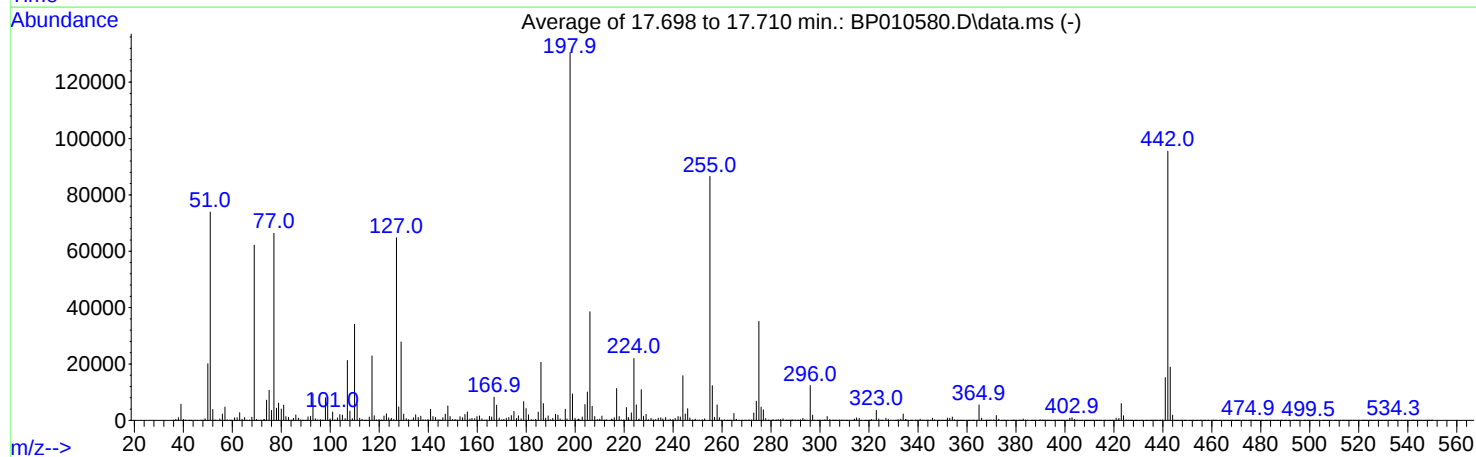


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010580.D
 Acq On : 27 May 2022 20:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 28 02:18:04 2022

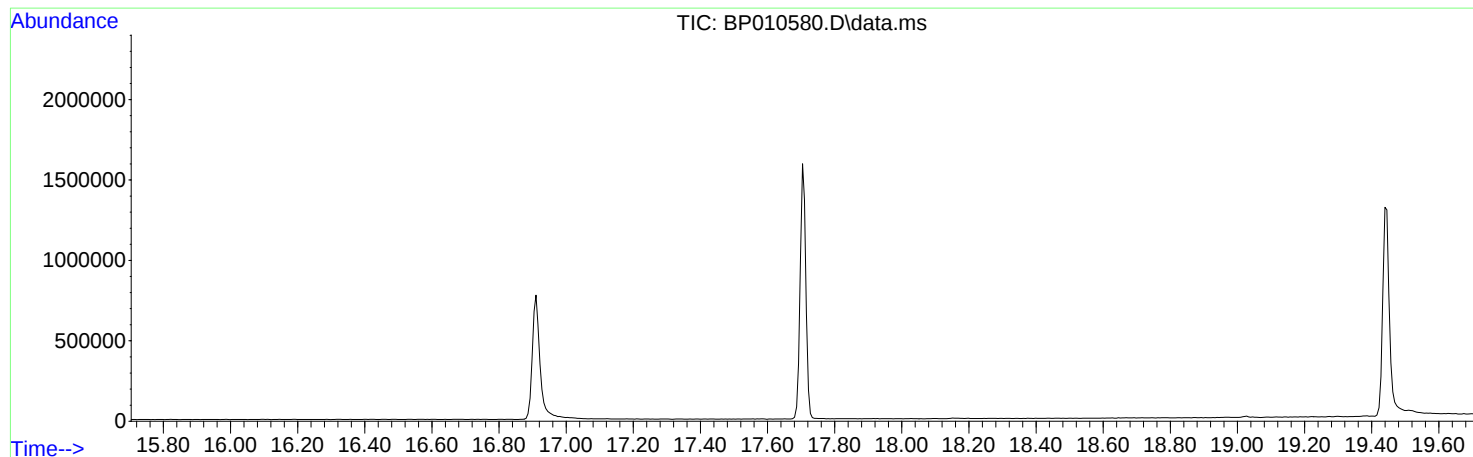


AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	73915	PASS
68	69	0.00	2	1.8	1125	PASS
69	198	0.00	100	47.6	62180	PASS
70	69	0.00	2	0.5	324	PASS
127	198	10	80	49.6	64755	PASS
197	198	0.00	2	0.4	515	PASS
198	198	100	100	100.0	130515	PASS
199	198	5	9	7.2	9383	PASS
275	198	10	60	26.9	35135	PASS
365	198	1	100	4.2	5525	PASS
441	198	0.01	100	11.6	15152	PASS
442	442	100	100	100.0	95501	PASS
443	442	15	24	19.8	18907	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010580.D
Acq On : 27 May 2022 20:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 05:18:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

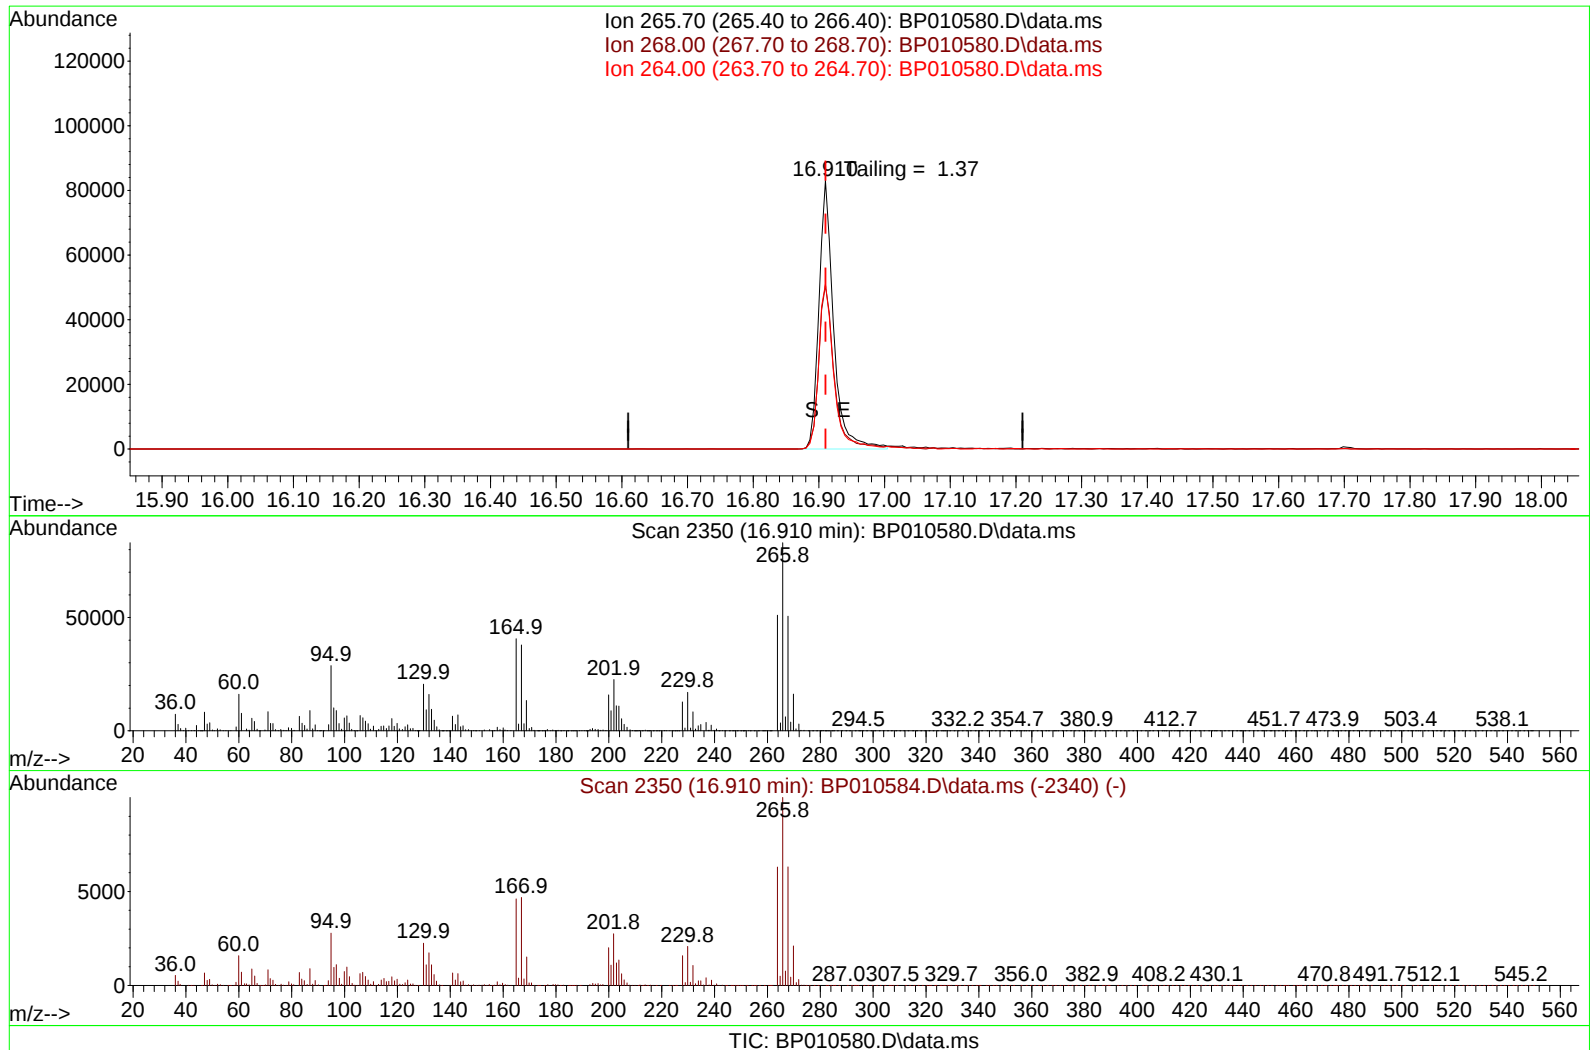

TIC: BP010580.D\data.ms

(70) Pentachlorophenol (C)

16.910min (+ 0.000) 827206.29 ng




response 131236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.94
264.00	63.00	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010580.D
Acq On : 27 May 2022 20:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 05:18:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

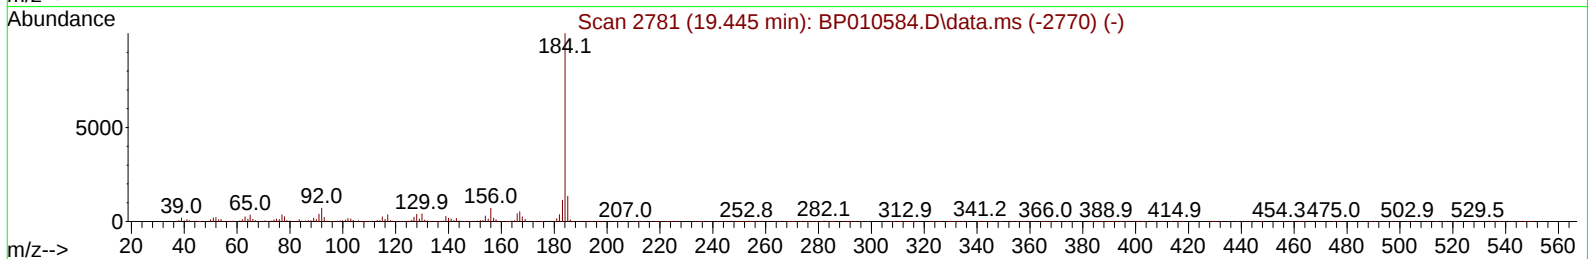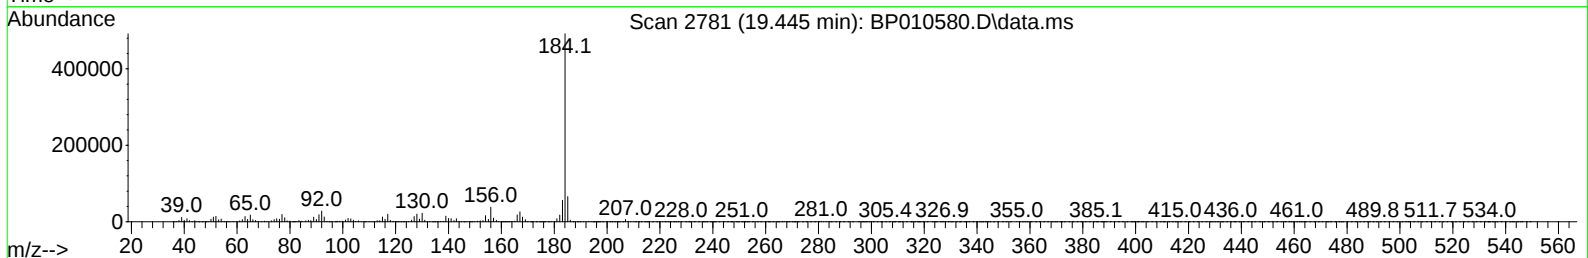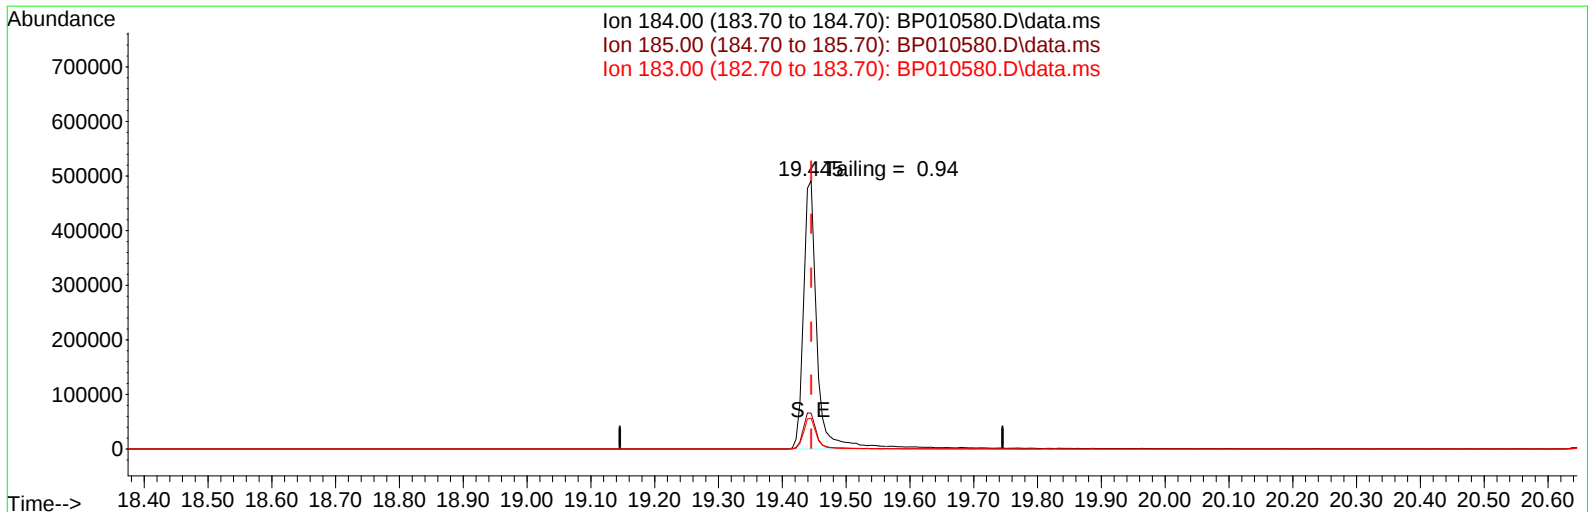

TIC: BP010580.D\data.ms

(77) Benzidine

19.445min (-0.000) 517946.55 ng

response 736257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.36
183.00	11.30	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2022	BNA_P	<u>BP010580.D</u>
Compound Name	Response	Retention Time
DDT	451747	20.645
DDD	2673	20.263
DDE	343	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3016	454763	0.66

Instrument :
BNA_P
ClientSampleId :
DFTPP