
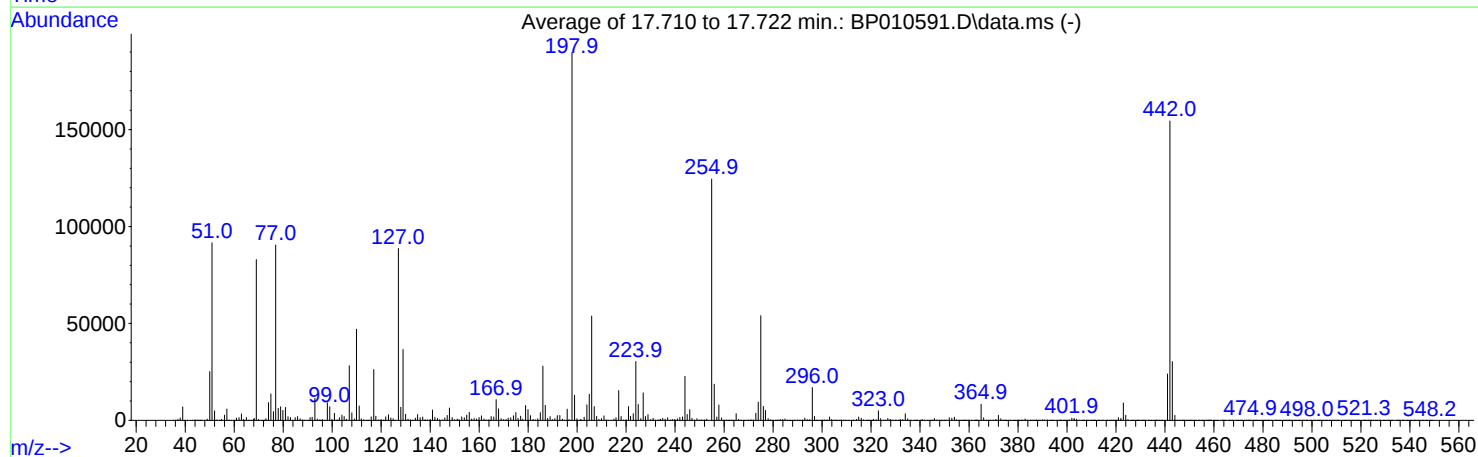


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010591.D
 Acq On : 28 May 2022 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 28 02:18:04 2022

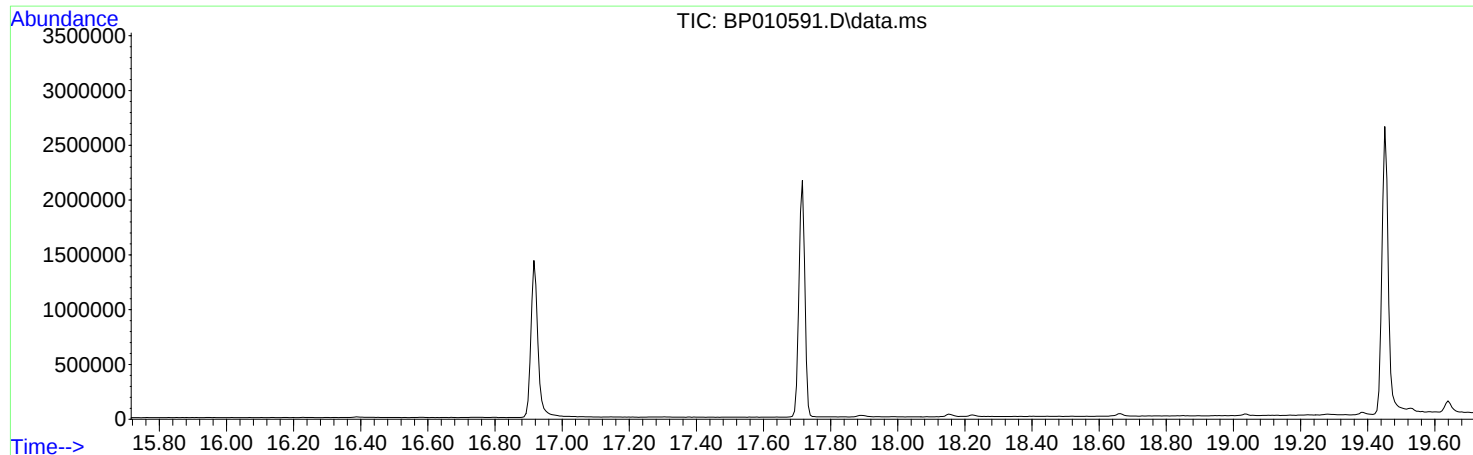




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	91631	PASS
68	69	0.00	2	1.2	1027	PASS
69	198	0.00	100	43.7	82945	PASS
70	69	0.00	2	0.6	512	PASS
127	198	10	80	46.7	88687	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	189773	PASS
199	198	5	9	6.8	12981	PASS
275	198	10	60	28.5	53997	PASS
365	198	1	100	4.4	8334	PASS
441	198	0.01	100	12.6	23923	PASS
442	442	100	100	100.0	154410	PASS
443	442	15	24	19.6	30293	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
 Data File : BP010591.D
 Acq On : 28 May 2022 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 29 04:44:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

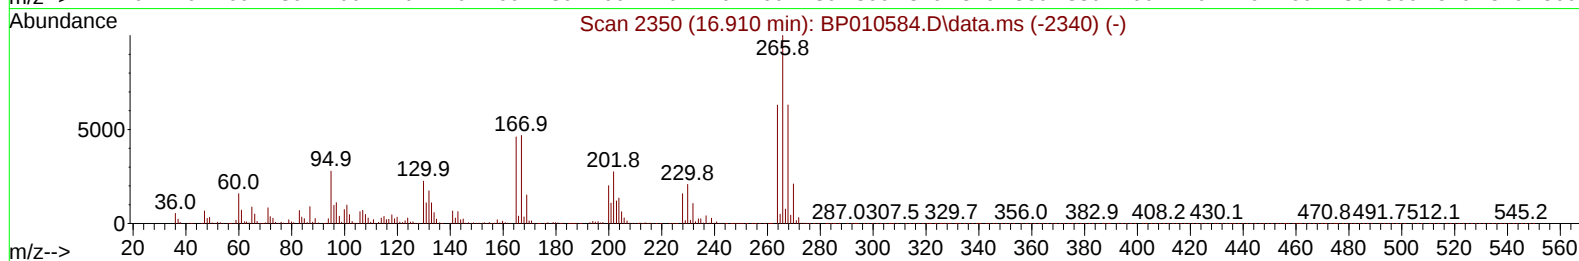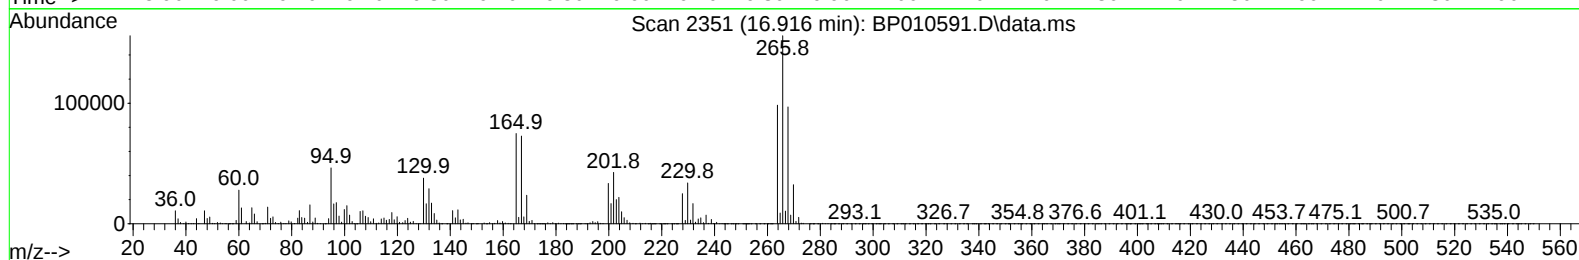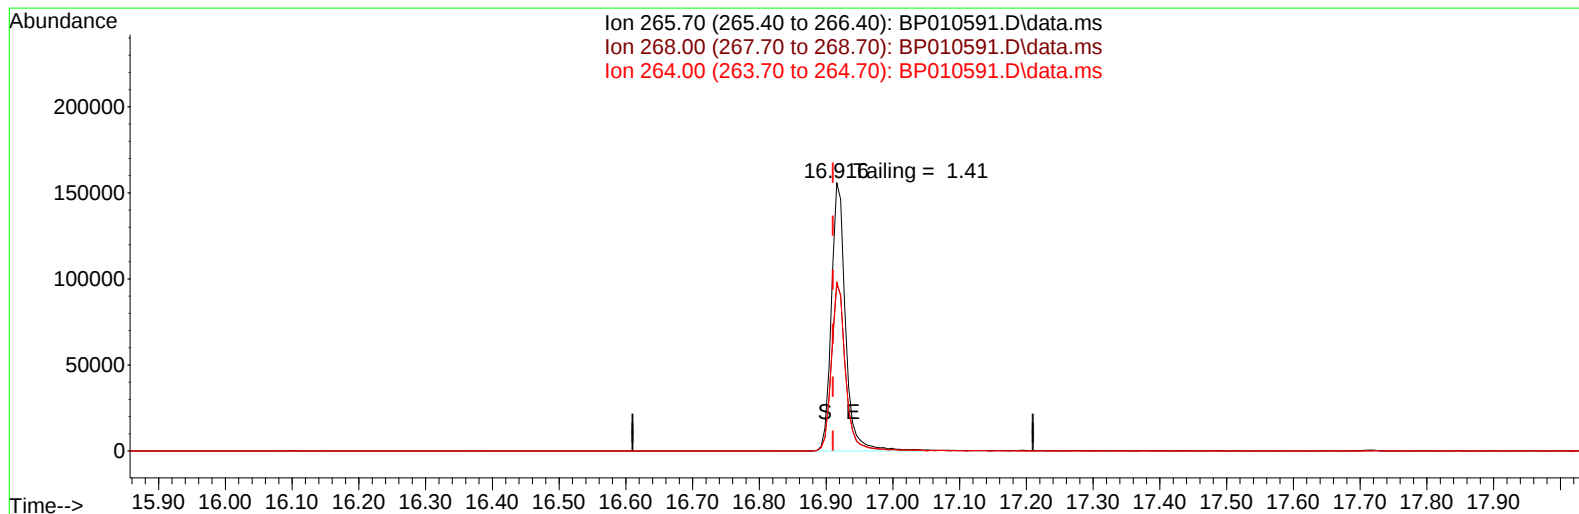

TIC: BP010591.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 208856.10 ng




response 230504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.15
264.00	63.00	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052822\
Data File : BP010591.D
Acq On : 28 May 2022 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 29 04:44:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

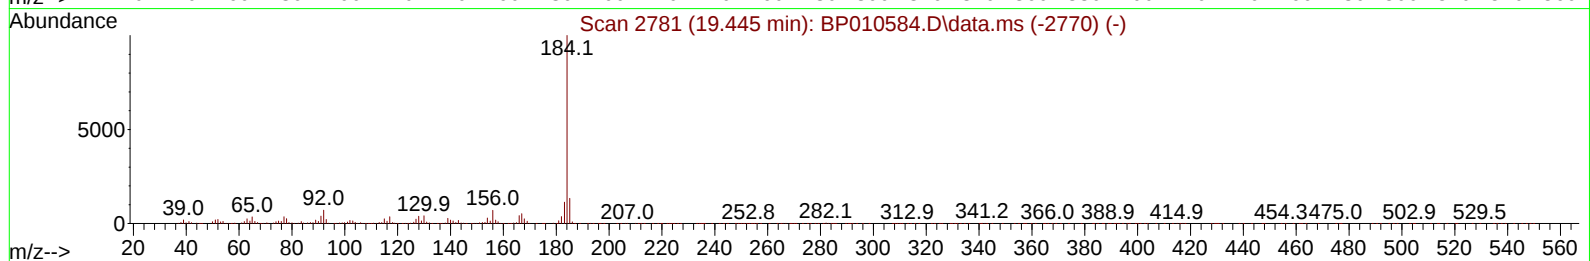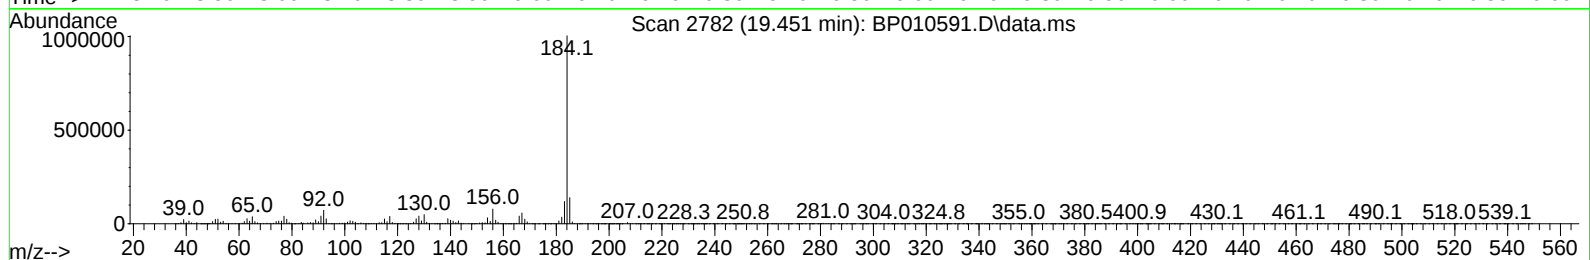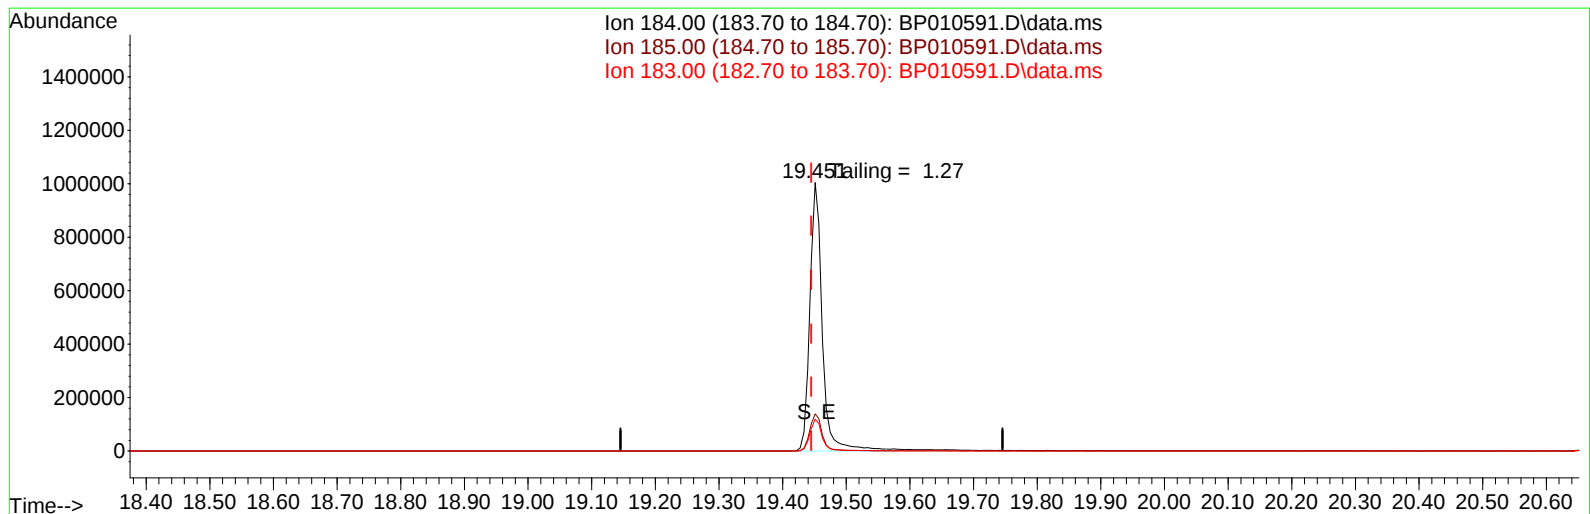

TIC: BP010591.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 20319.56 ng

response 1386046

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.85
183.00	11.30	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2022	BNA_P	<u>BP010591.D</u>
Compound Name	Response	Retention Time
DDT	748541	20.657
DDD	7449	20.228
DDE	879	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8328	756869	1.10

Instrument :
BNA_P
ClientSampleId :
DFTPP