
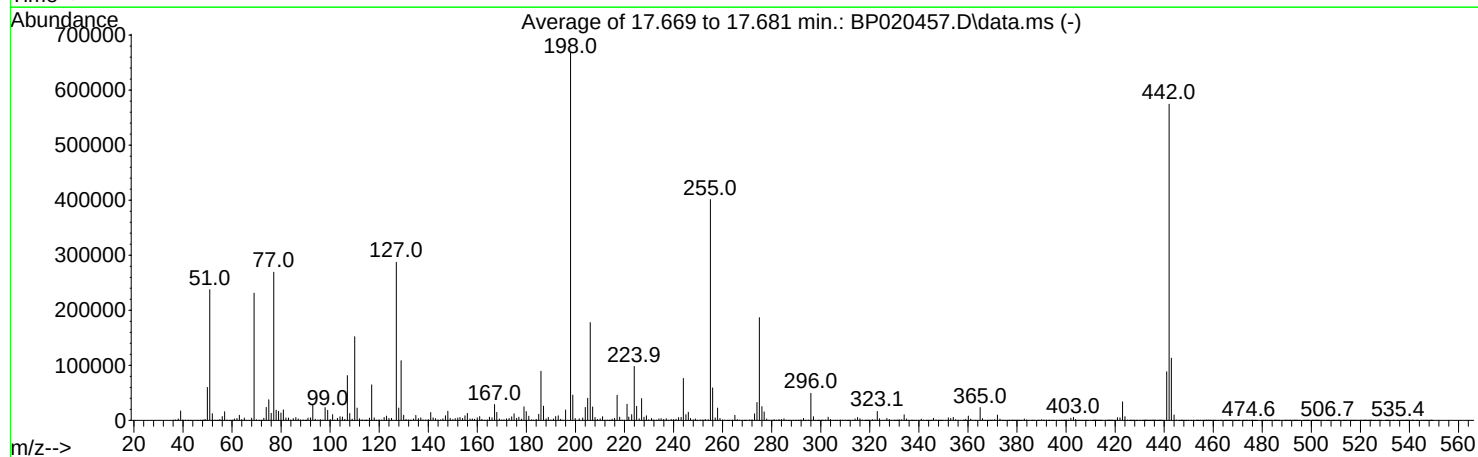


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052824\
Data File : BP020457.D
Acq On : 28 May 2024 11:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 29 01:36:38 2024

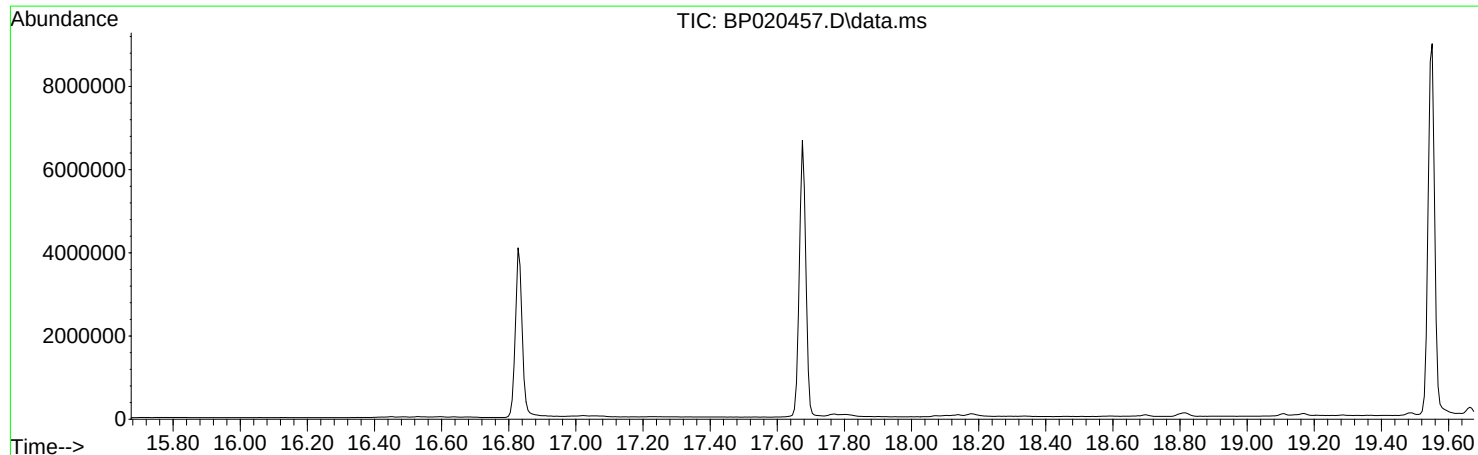




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	237455	PASS
68	69	0.00	2	1.7	4020	PASS
69	198	0.00	100	34.6	230977	PASS
70	69	0.00	2	0.5	1114	PASS
127	198	10	80	43.0	287130	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	668319	PASS
199	198	5	9	6.9	45949	PASS
275	198	10	60	27.9	186603	PASS
365	198	1	100	3.5	23232	PASS
441	198	0.01	100	13.2	88298	PASS
442	442	100	100	100.0	574272	PASS
443	442	15	24	19.7	113122	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052824\
Data File : BP020457.D
Acq On : 28 May 2024 11:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 12:25:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 25 02:22:23 2024
Response via : Initial Calibration

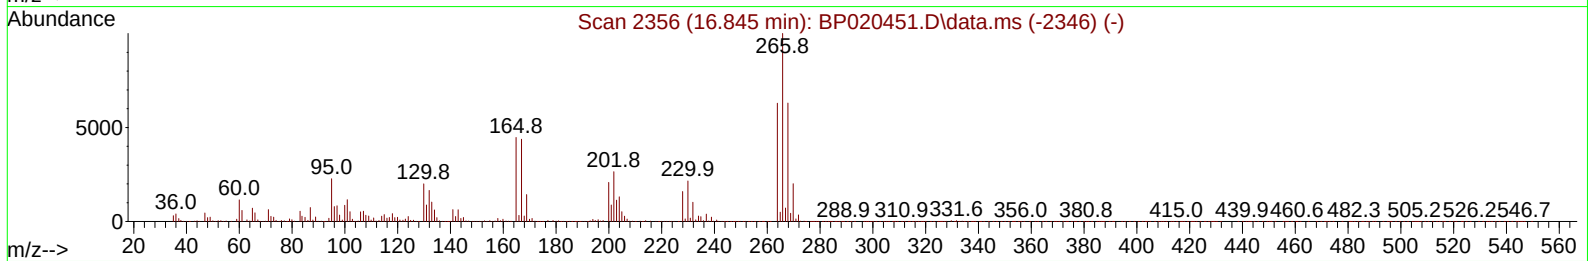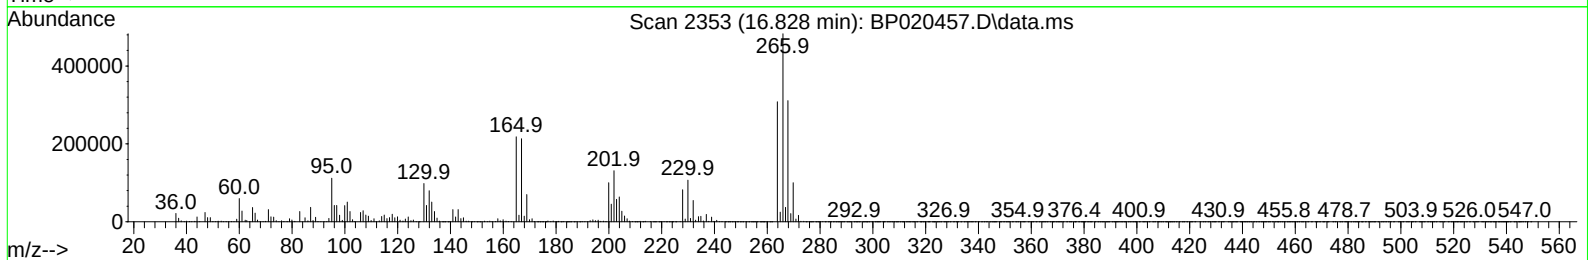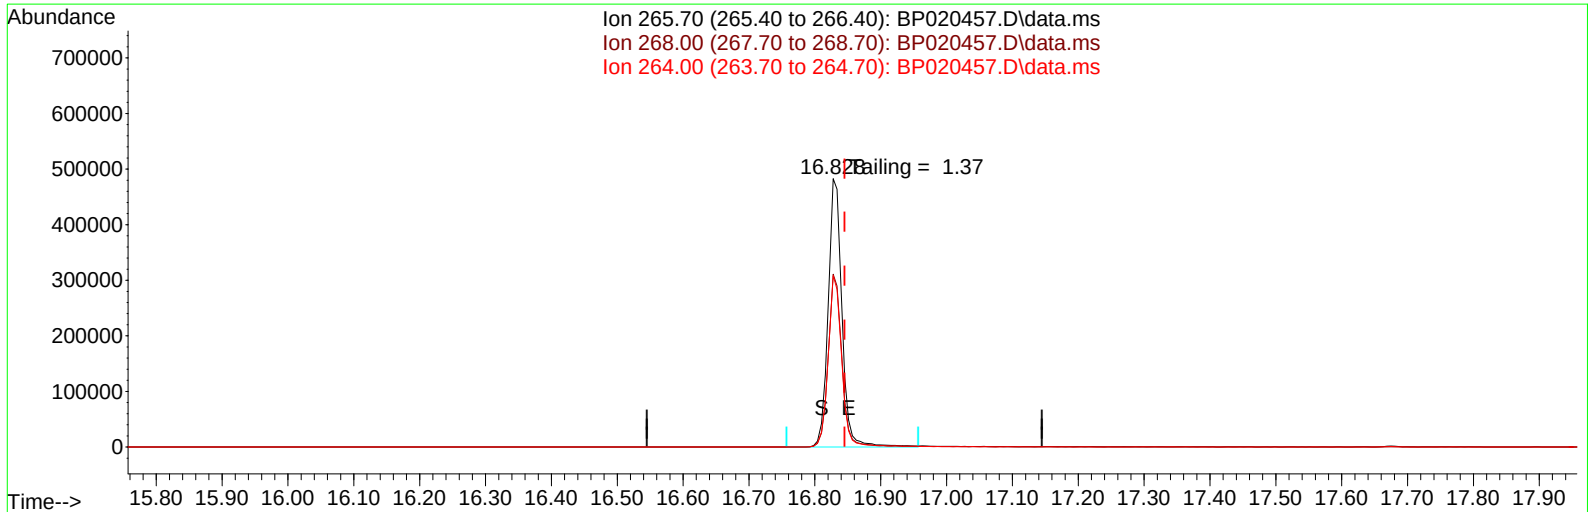

TIC: BP020457.D\data.ms

(70) Pentachlorophenol (C)

16.828min (-0.017) 6935405.96 ng




response 703665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.40
264.00	62.90	63.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052824\
Data File : BP020457.D
Acq On : 28 May 2024 11:13
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 28 12:25:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 25 02:22:23 2024
Response via : Initial Calibration

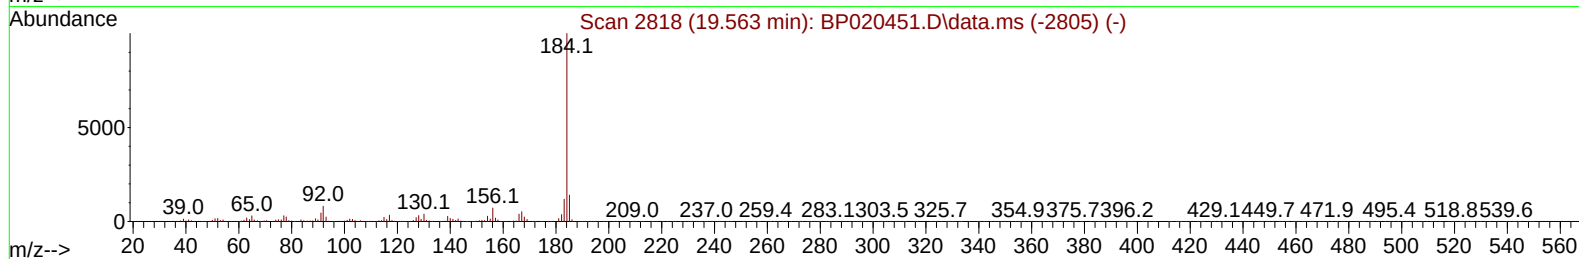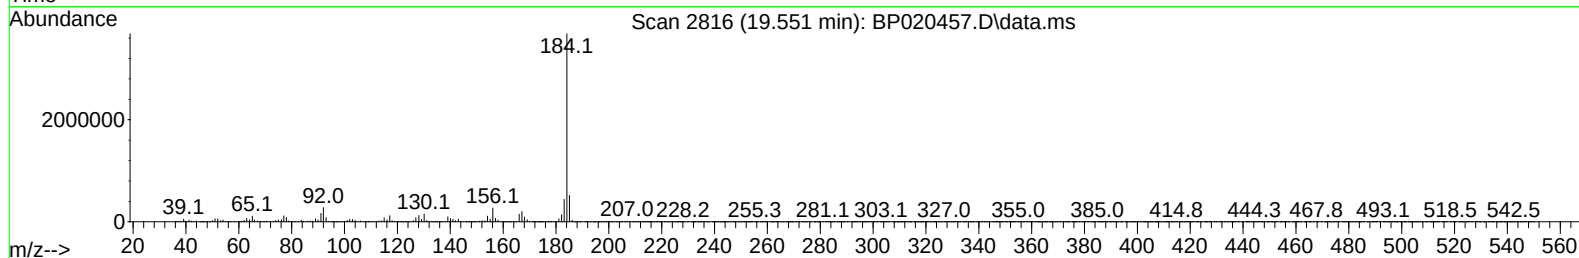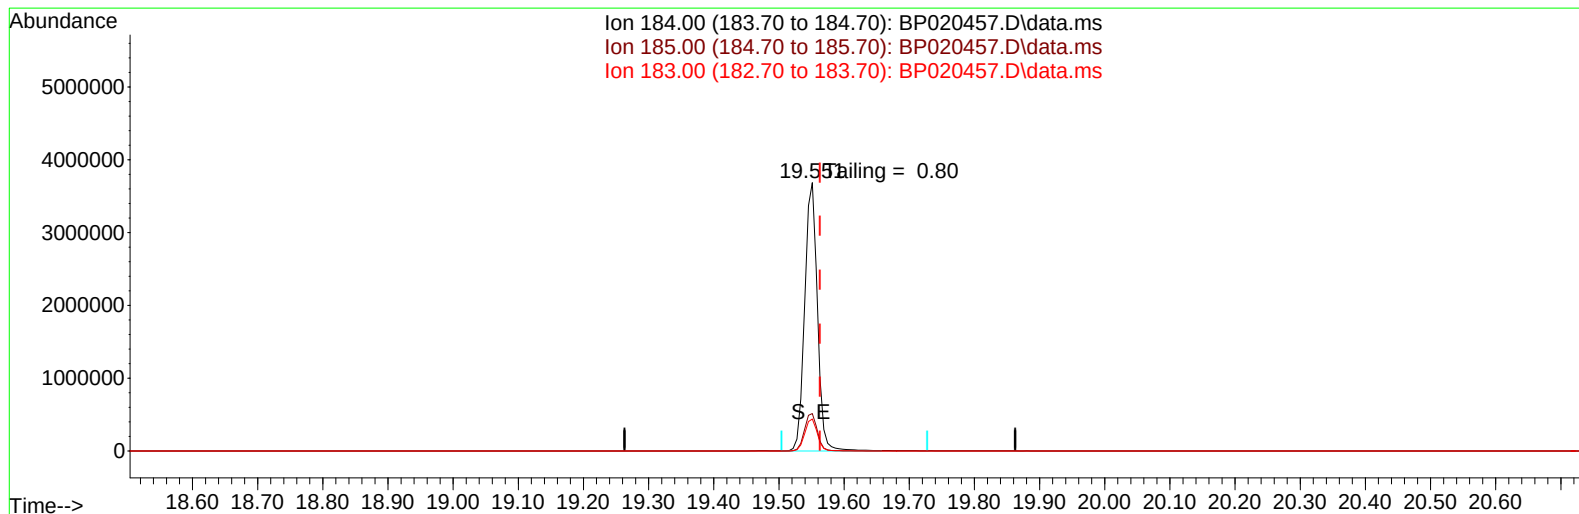

TIC: BP020457.D\data.ms

(77) Benzidine

19.551min (-0.012) -20.00 ng

response 4987423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.98
183.00	11.80	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2024	BNA_P	<u>BP020457.D</u>
Compound Name	Response	Retention Time
DDT	2216568	20.851
DDD	28737	20.439
DDE	2066	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30803	2247371	1.37

Instrument :
BNA_P
ClientSampleId :
DFTPP