
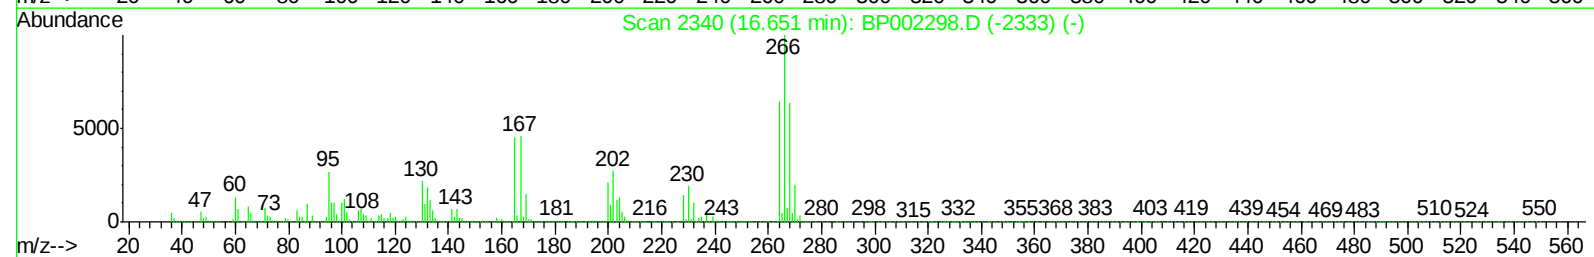
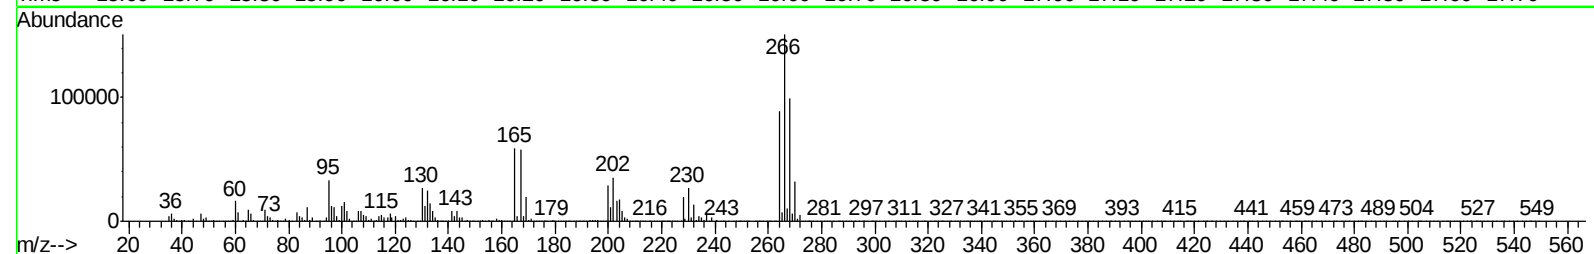


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP052920\
 Data File : BP002313.D
 Acq On : 29 May 2020 13:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 03:05:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 15:09:03 2020
 Response via : Initial Calibration

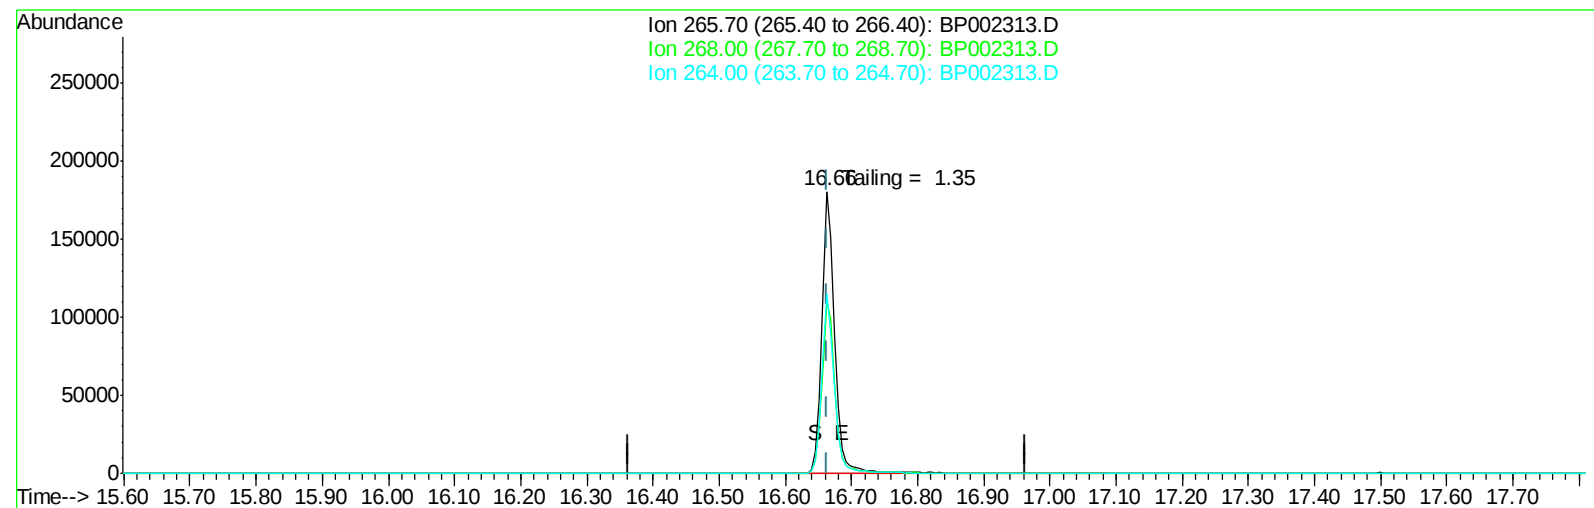

TIC: BP002313.D

(70) Pentachlorophenol (C)




16.663min (+0.000) 2777410.75ng

response 246284

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	60.70
264.00	60.40	63.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP052920\
 Data File : BP002313.D
 Acq On : 29 May 2020 13:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 03:05:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 15:09:03 2020
 Response via : Initial Calibration

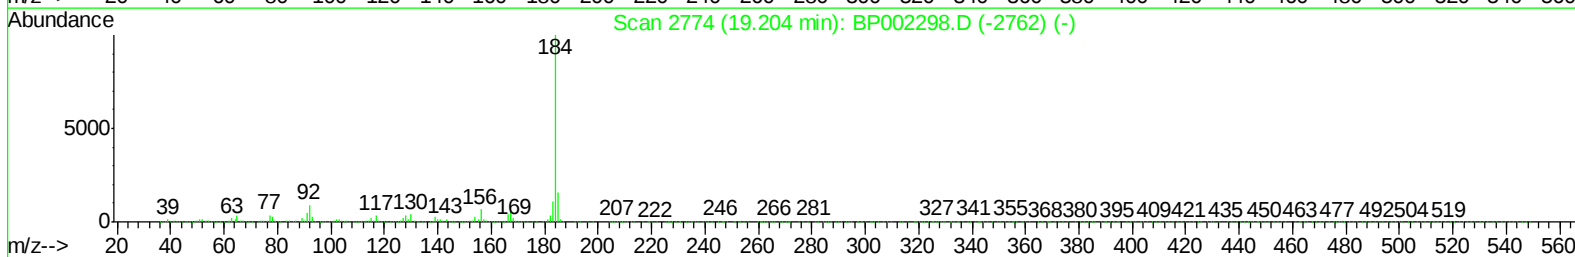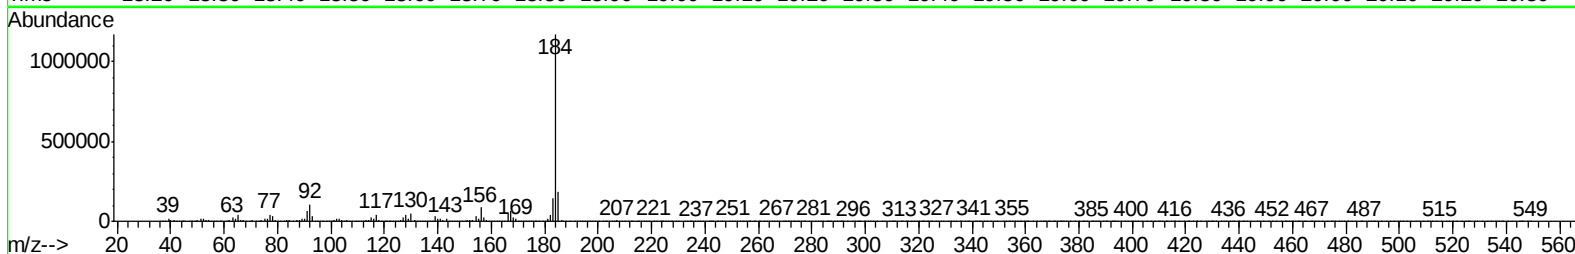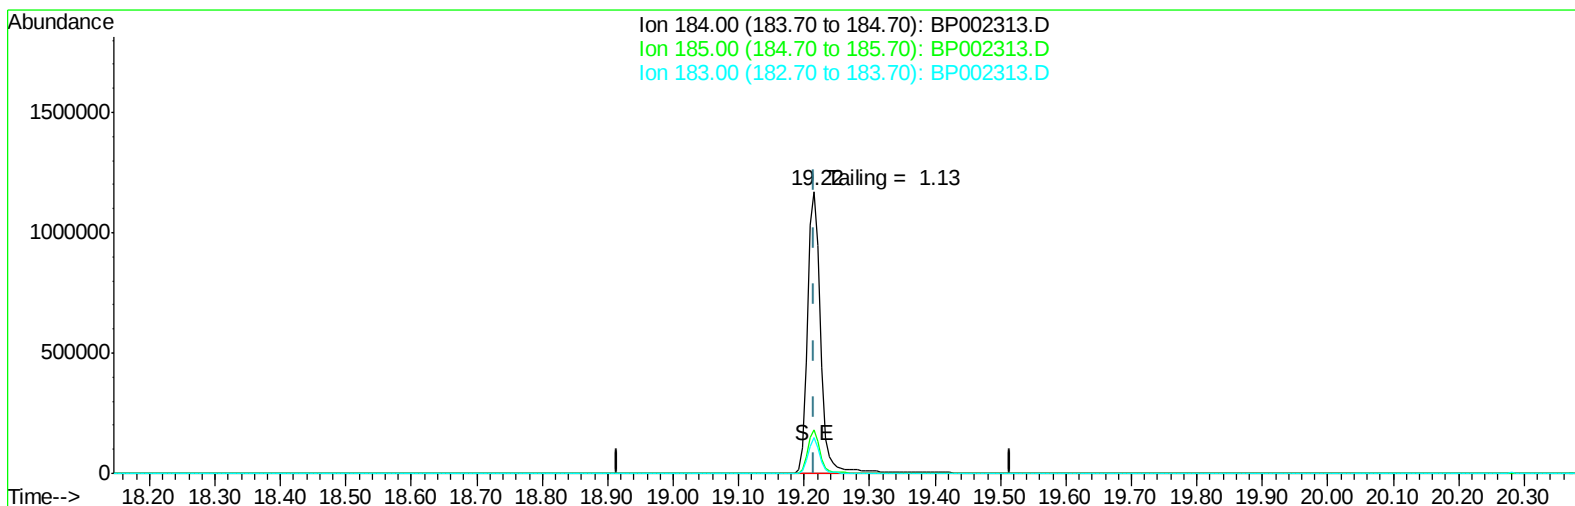

TIC: BP002313.D

(77) Benzidine

19.216min (+0.000) 200658.69ng

response 1650332

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.64
183.00	11.40	12.67
0.00	0.00	0.00