


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP052920\
 Data File : BP002313.D
 Acq On : 29 May 2020 13:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 29 15:09:03 2020

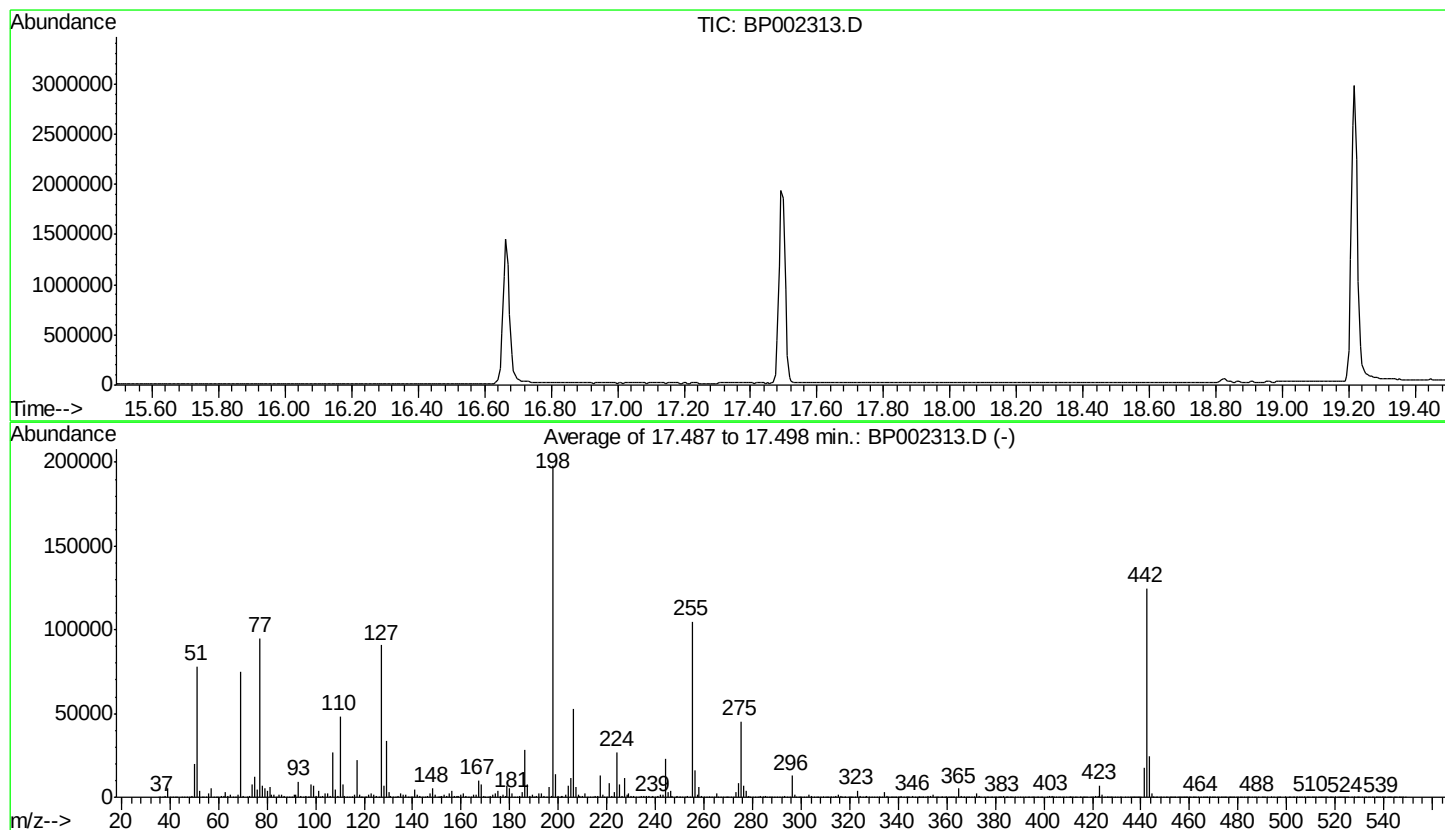

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	78176	PASS
68	69	0.00	2	1.7	1272	PASS
69	198	0.00	100	38.0	75282	PASS
70	69	0.00	2	0.6	451	PASS
127	198	10	80	45.8	90771	PASS
197	198	0.00	2	0.5	899	PASS
198	198	100	100	100.0	198047	PASS
199	198	5	9	7.0	13887	PASS
275	198	10	60	22.9	45302	PASS
365	198	1	100	2.6	5152	PASS
441	198	0.01	100	9.0	17851	PASS
442	198	50	100	63.0	124680	PASS
443	442	15	24	19.6	24440	PASS