

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010620.D
Acq On : 29 May 2022 15:47
Operator : CG/JU
Sample : N2951-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS002-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	412	rBV	1803047	2664176	12.67%	5.589%
2	7.040	662	672	688	rBV	1711737	2808137	13.35%	5.891%
3	7.863	806	812	821	rBV	421140	685240	3.26%	1.437%
4	9.028	1002	1010	1025	rBV	1024231	1825040	8.68%	3.828%
5	10.669	1279	1289	1302	rBV	503699	934339	4.44%	1.960%
6	13.122	1699	1706	1729	rBV	2341016	3703623	17.61%	7.769%
7	14.498	1932	1940	1951	rBV	727226	1169753	5.56%	2.454%
8	15.992	2188	2194	2213	rBV	1809400	2749014	13.07%	5.767%
9	17.257	2403	2409	2415	rBV	853817	1307629	6.22%	2.743%
10	19.810	2838	2843	2854	rBV	4091135	5018165	23.86%	10.527%
11	21.051	3050	3054	3062	rBV	588506	771274	3.67%	1.618%
12	21.339	3099	3103	3109	rBV	1070744	1360098	6.47%	2.853%
13	21.463	3117	3124	3145	rBV	13815493	21035382	100.00%	44.126%
14	21.780	3175	3178	3184	rVB	154903	210852	1.00%	0.442%
15	23.751	3507	3513	3522	rVB2	695974	1427950	6.79%	2.995%




Sum of corrected areas: 47670672

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010620.D
Acq On : 29 May 2022 15:47
Operator : CG/JU
Sample : N2951-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

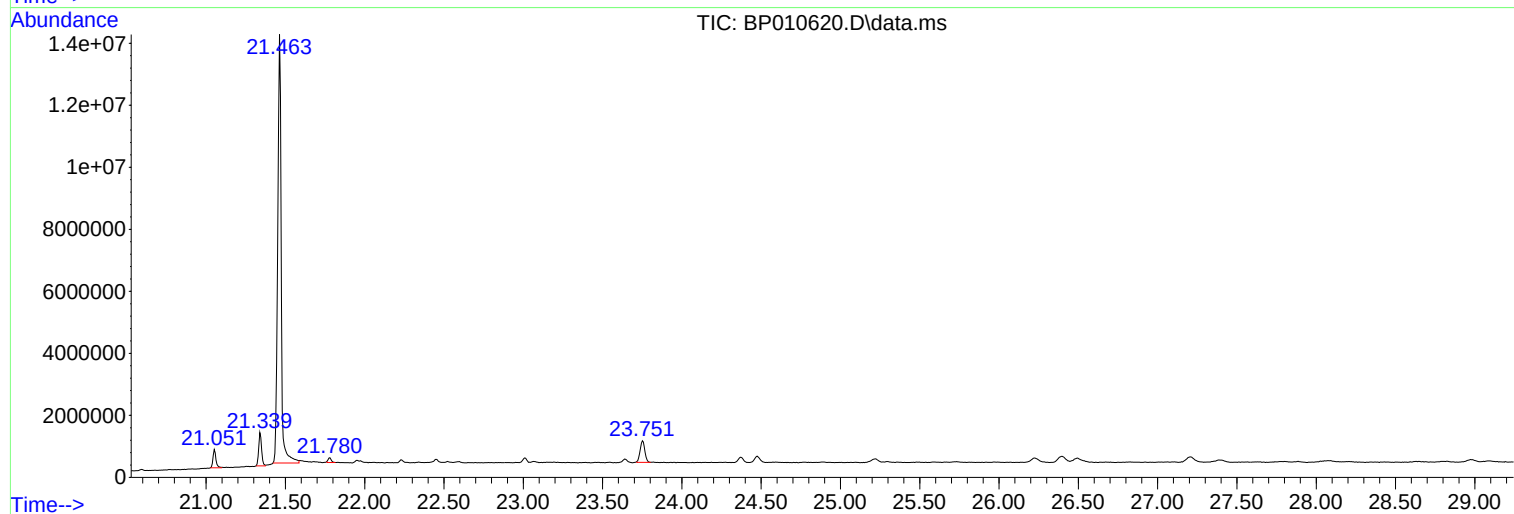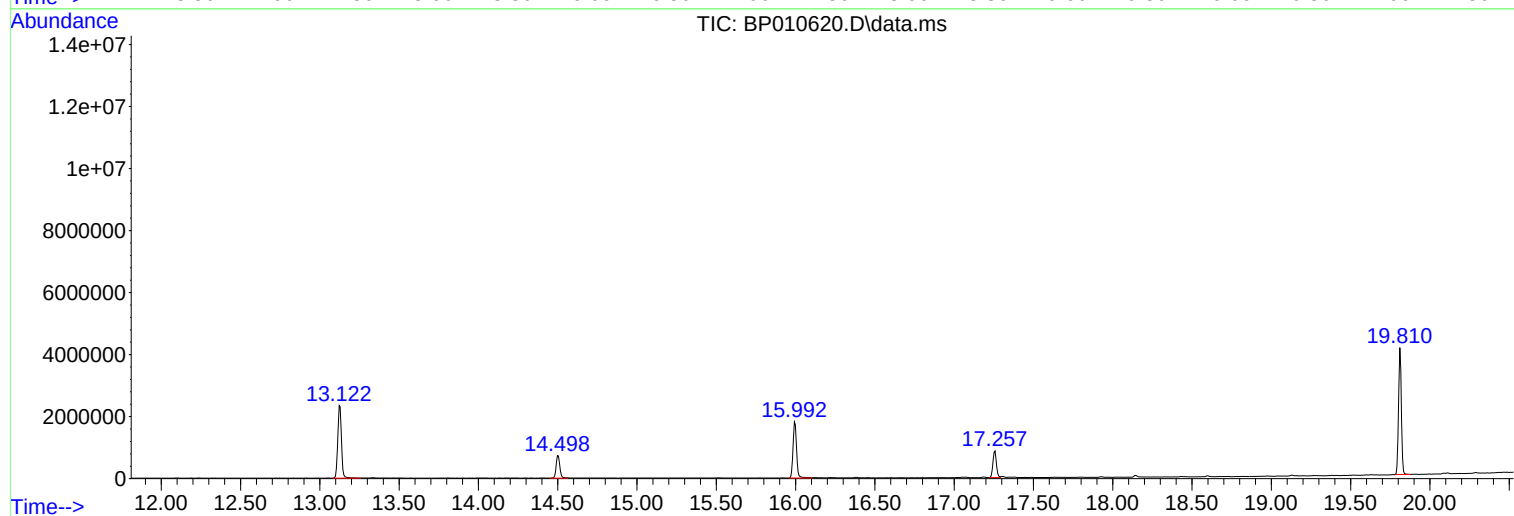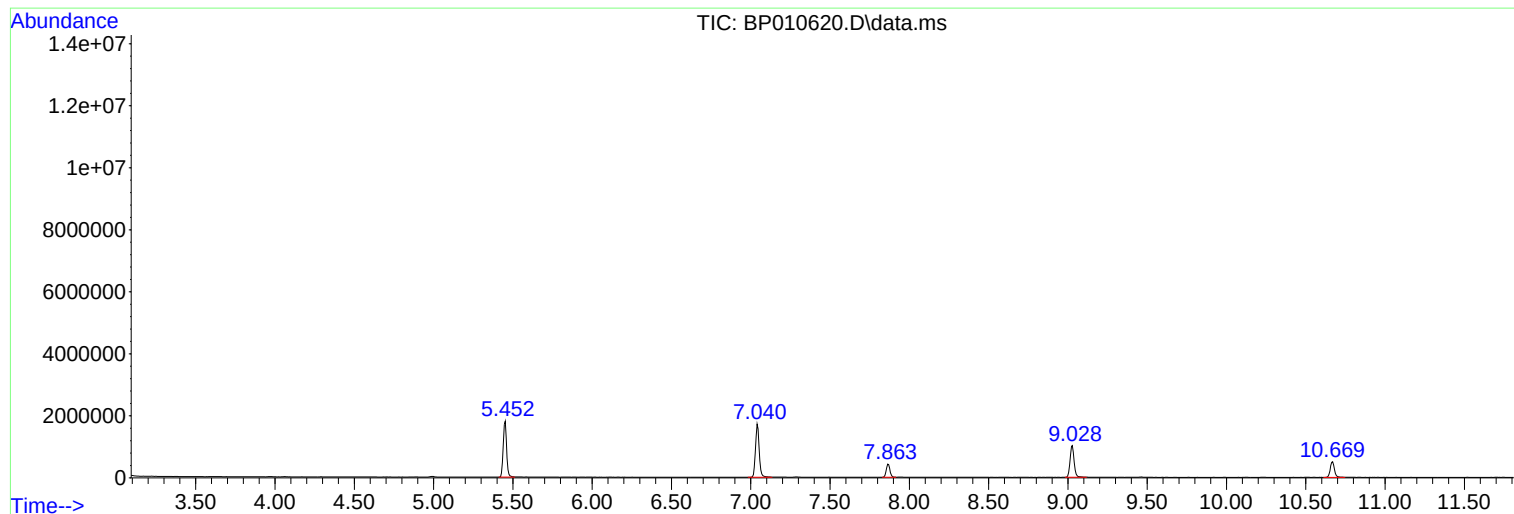

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010620.D
Acq On : 29 May 2022 15:47
Operator : CG/JU
Sample : N2951-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010620.D
Acq On : 29 May 2022 15:47
Operator : CG/JU
Sample : N2951-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS002-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc