

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
 Data File : BP010621.D
 Acq On : 29 May 2022 16:20
 Operator : CG/JU
 Sample : N2951-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P035-SS001-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	414	rBV	1788525	2703383	13.29%	5.764%
2	7.040	665	672	690	rBV	1728500	2830126	13.92%	6.034%
3	7.863	806	812	821	rBV	453437	733746	3.61%	1.564%
4	9.028	1002	1010	1026	rBV	1051745	1868864	9.19%	3.985%
5	10.669	1280	1289	1299	rBV	537387	985077	4.84%	2.100%
6	13.122	1699	1706	1729	rBV	2276581	3466802	17.05%	7.392%
7	14.504	1933	1941	1953	rBV	767139	1245695	6.13%	2.656%
8	15.992	2187	2194	2211	rBV	1866188	2802697	13.78%	5.976%
9	17.257	2402	2409	2423	rBV	947362	1414225	6.95%	3.015%
10	19.810	2838	2843	2851	rBV	3931142	4689311	23.06%	9.998%
11	21.051	3050	3054	3061	rBV	391724	522520	2.57%	1.114%
12	21.339	3098	3103	3109	rBV	1202179	1545881	7.60%	3.296%
13	21.463	3117	3124	3147	rBV	14135476	20335835	100.00%	43.359%
14	21.774	3175	3177	3185	rVB	155090	204827	1.01%	0.437%
15	23.751	3507	3513	3524	rVB2	786226	1552221	7.63%	3.310%




Sum of corrected areas: 46901210

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010621.D
Acq On : 29 May 2022 16:20
Operator : CG/JU
Sample : N2951-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

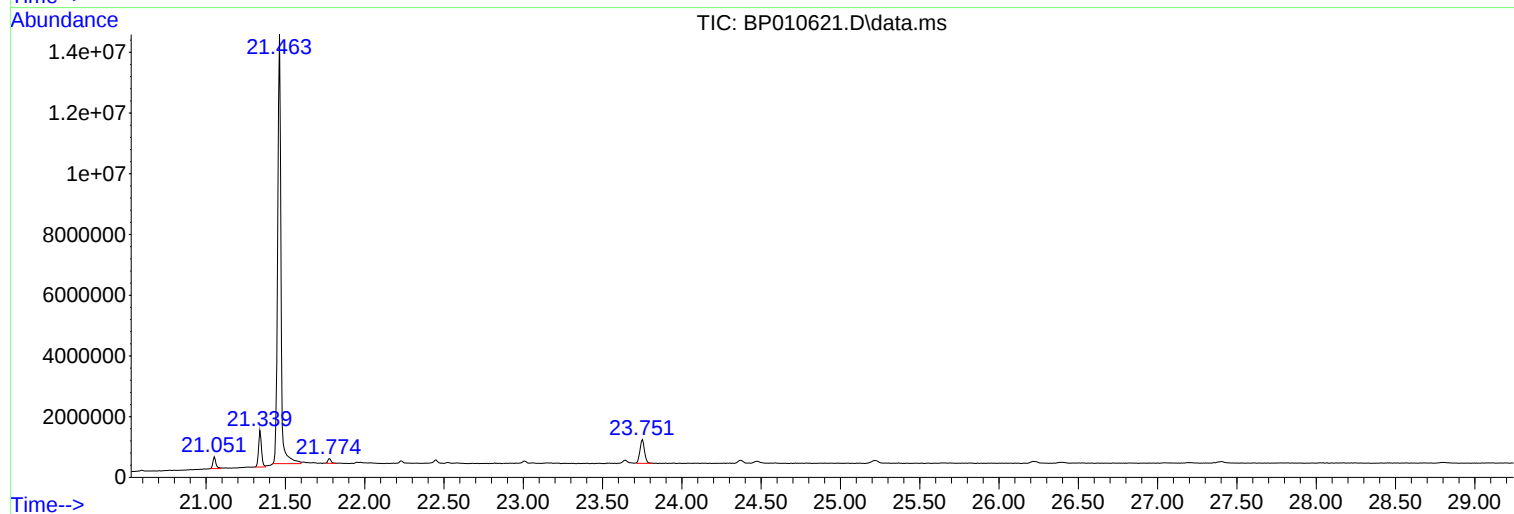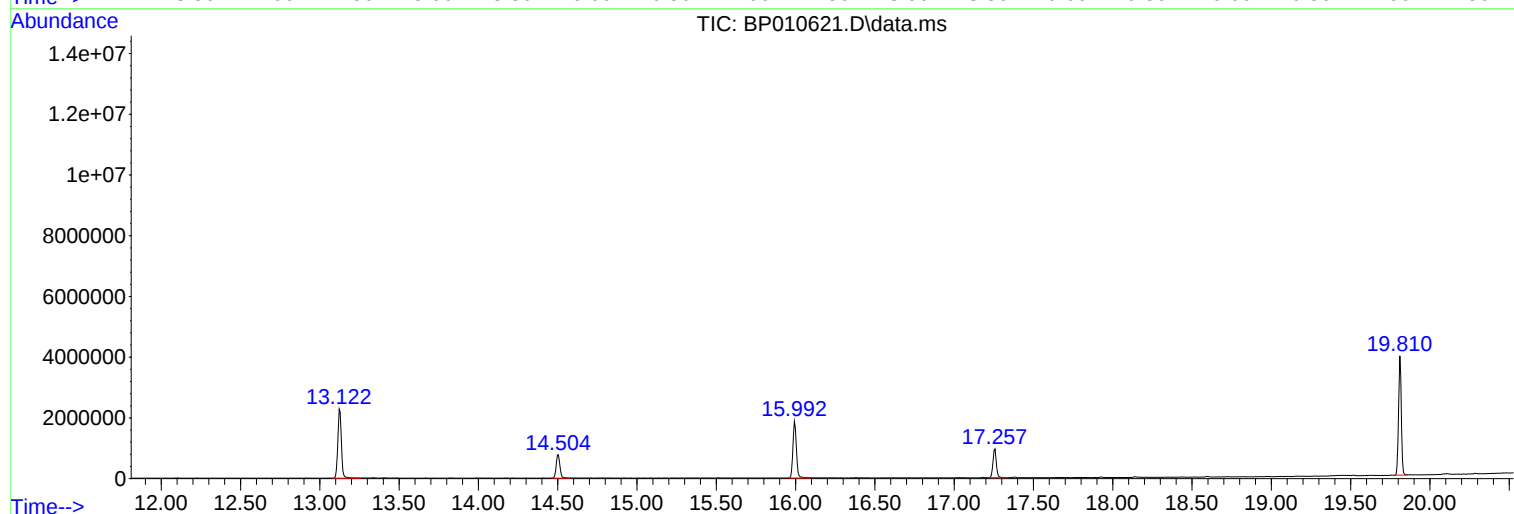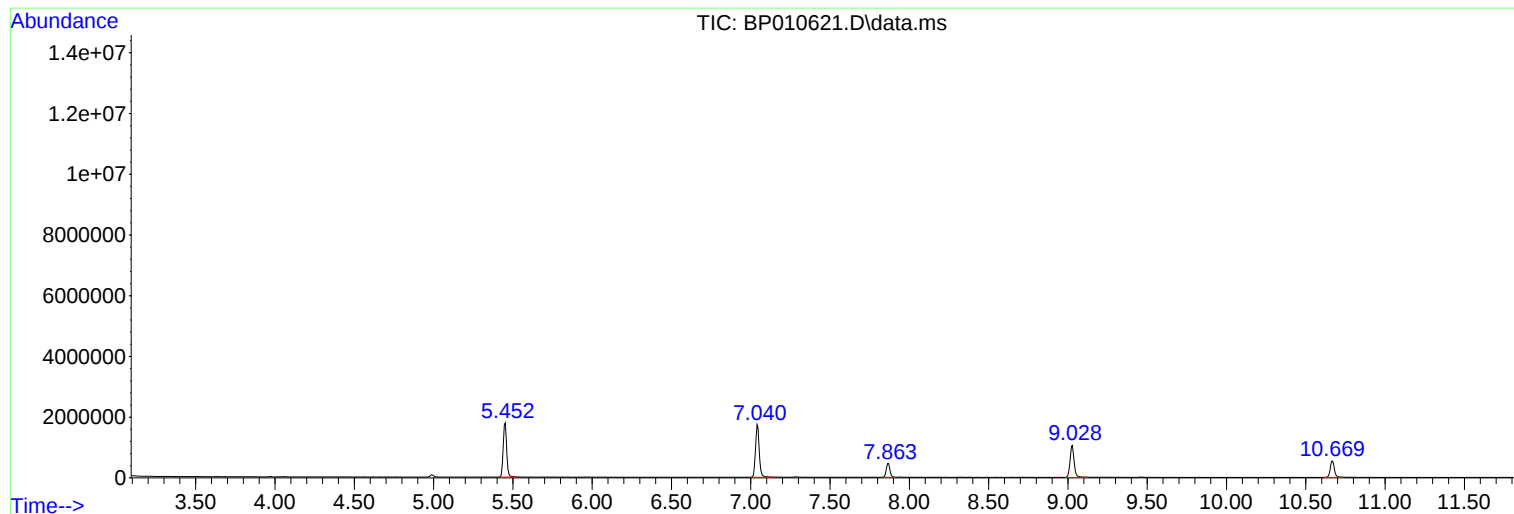

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010621.D
Acq On : 29 May 2022 16:20
Operator : CG/JU
Sample : N2951-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010621.D
Acq On : 29 May 2022 16:20
Operator : CG/JU
Sample : N2951-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P035-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc