

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
 Data File : BP010624.D
 Acq On : 29 May 2022 18:02
 Operator : CG/JU
 Sample : N2932-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P016-SS004-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	416	rBV	2447809	3623792	19.42%	6.707%
2	7.040	663	672	687	rBV	2244884	3768721	20.20%	6.975%
3	7.863	805	812	821	rBV	531720	853597	4.57%	1.580%
4	9.028	1002	1010	1023	rBV	1403781	2463882	13.20%	4.560%
5	10.663	1280	1288	1299	rBV	638522	1135185	6.08%	2.101%
6	13.128	1699	1707	1726	rBV	3292566	5070676	27.17%	9.385%
7	14.498	1932	1940	1954	rBV	902886	1434981	7.69%	2.656%
8	15.992	2187	2194	2214	rBV	2388647	3670194	19.67%	6.793%
9	17.257	2402	2409	2420	rBV	1073459	1571363	8.42%	2.908%
10	18.145	2555	2560	2569	rBV	172464	270530	1.45%	0.501%
11	19.810	2838	2843	2852	rBV	5369368	6490597	34.78%	12.013%
12	21.051	3049	3054	3063	rBV2	723542	1043331	5.59%	1.931%
13	21.245	3084	3087	3092	rBV	458320	524637	2.81%	0.971%
14	21.339	3098	3103	3112	rBV	1259112	1778196	9.53%	3.291%
15	21.463	3117	3124	3142	rVV	12381620	18660102	100.00%	34.538%
16	23.751	3507	3513	3521	rVB	830847	1668433	8.94%	3.088%




Sum of corrected areas: 54028217

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010624.D
Acq On : 29 May 2022 18:02
Operator : CG/JU
Sample : N2932-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

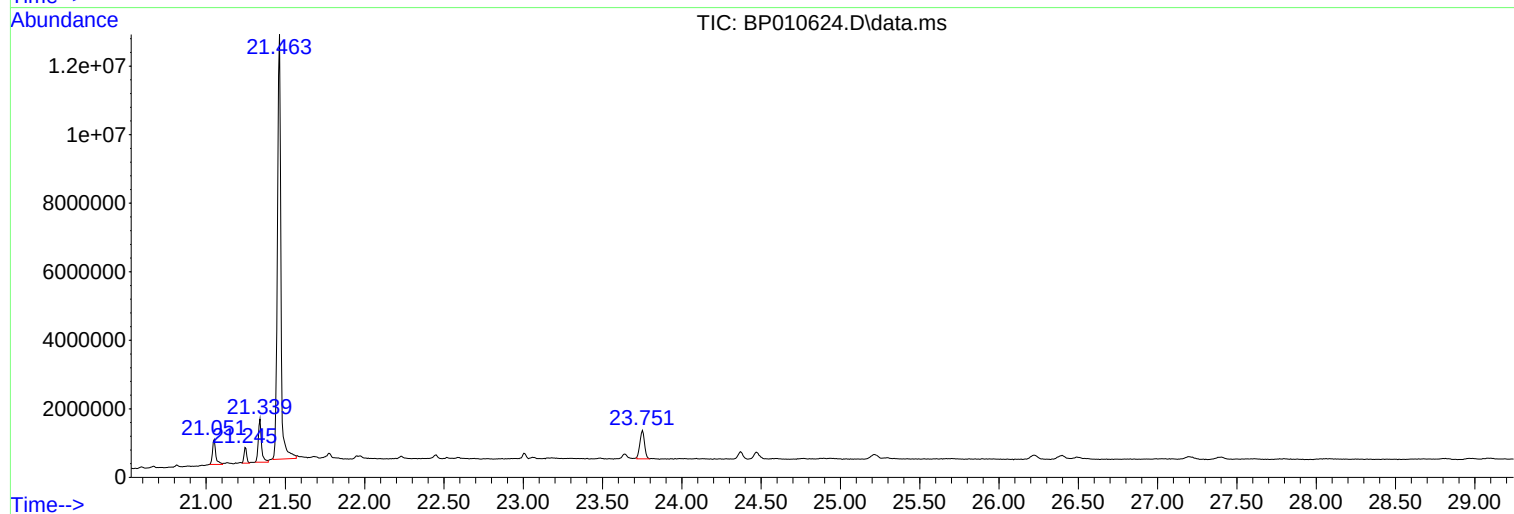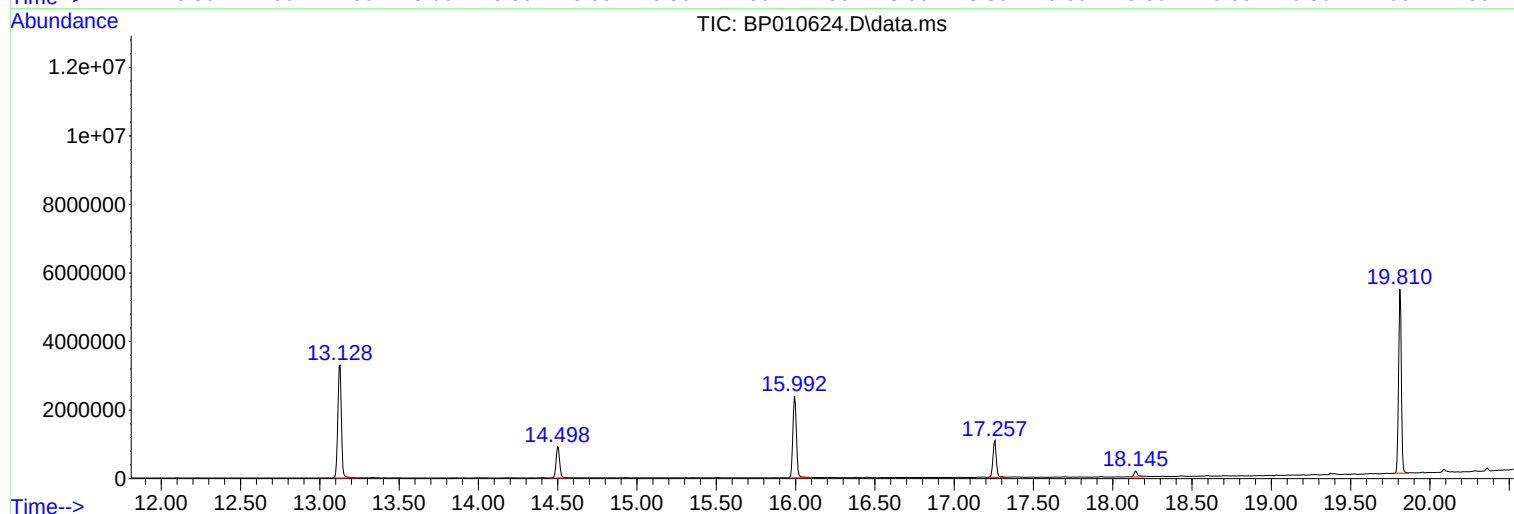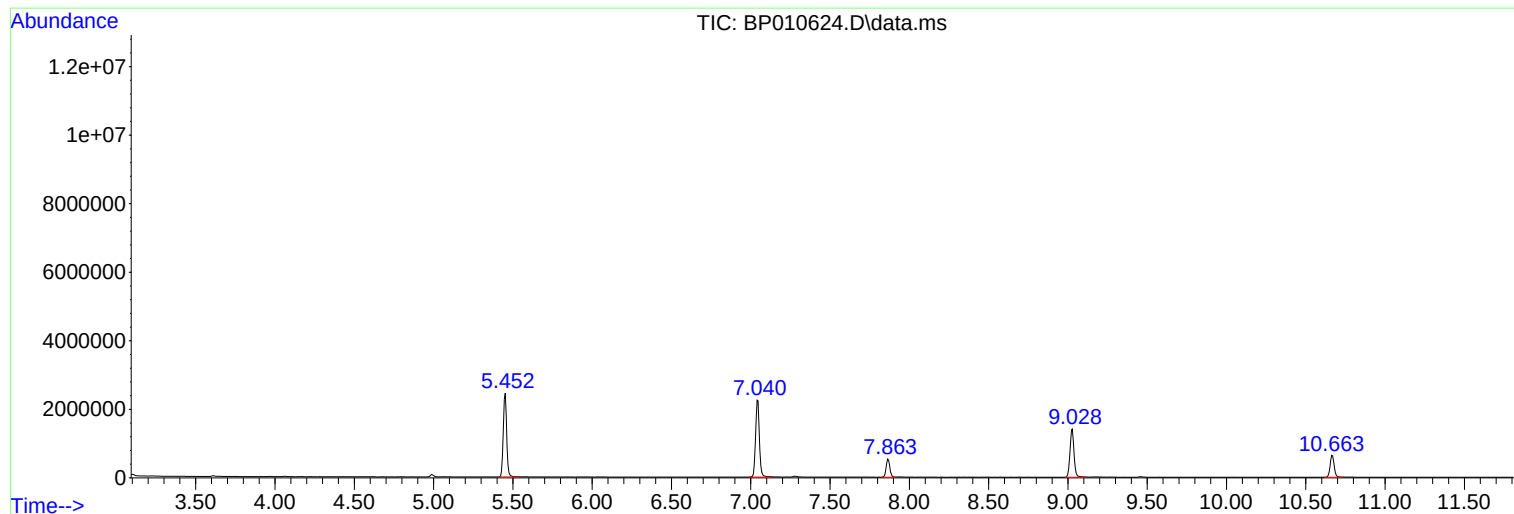

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010624.D
Acq On : 29 May 2022 18:02
Operator : CG/JU
Sample : N2932-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010624.D
Acq On : 29 May 2022 18:02
Operator : CG/JU
Sample : N2932-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P016-SS004-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc