

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
 Data File : BP010626.D
 Acq On : 29 May 2022 19:10
 Operator : CG/JU
 Sample : N2928-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 P026-SS001-1824-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.640	87	94	106	rBV2	66232	193454	1.32%	0.296%
2	5.452	395	402	410	rBV	1994842	2977142	20.31%	4.550%
3	7.046	663	673	680	rBV	1914348	3235380	22.07%	4.945%
4	7.134	684	688	696	rVB	100004	173777	1.19%	0.266%
5	7.863	805	812	817	rBV	534003	853333	5.82%	1.304%
6	7.922	817	822	838	rVV5	192717	650823	4.44%	0.995%
7	9.022	1002	1009	1027	rVB	1263406	2170624	14.81%	3.318%
8	10.663	1281	1288	1301	rVB	700553	1209110	8.25%	1.848%
9	11.498	1417	1430	1438	rBV7	83704	289776	1.98%	0.443%
10	12.310	1563	1568	1577	rVB	114023	209579	1.43%	0.320%
11	12.446	1585	1591	1604	rBV	146125	467160	3.19%	0.714%
12	13.122	1700	1706	1718	rVB	3003772	4424016	30.18%	6.762%
13	13.263	1725	1730	1732	rBV3	106238	166256	1.13%	0.254%
14	14.163	1878	1883	1887	rBV3	94109	173253	1.18%	0.265%
15	14.498	1935	1940	1946	rBV	1004339	1484858	10.13%	2.269%
16	15.992	2188	2194	2200	rBV	2383955	3424579	23.37%	5.234%
17	16.057	2201	2205	2212	rVB2	113811	210148	1.43%	0.321%
18	16.222	2230	2233	2246	rVB4	65313	173107	1.18%	0.265%
19	16.798	2327	2331	2335	rVB2	159099	189654	1.29%	0.290%
20	17.251	2403	2408	2415	rVB	1195186	1690924	11.54%	2.584%
21	17.651	2472	2476	2480	rBV3	128484	203339	1.39%	0.311%
22	18.145	2557	2560	2566	rBV	382183	468993	3.20%	0.717%
23	18.251	2575	2578	2583	rBV	202444	243594	1.66%	0.372%
24	18.880	2682	2685	2690	rBV	218661	255637	1.74%	0.391%
25	19.457	2780	2783	2788	rVB	293464	336405	2.30%	0.514%
26	19.810	2839	2843	2849	rBV	4724300	5947595	40.58%	9.090%
27	19.957	2865	2868	2871	rBV	383251	397734	2.71%	0.608%
28	20.092	2888	2891	2897	rVB2	424580	507462	3.46%	0.776%
29	20.363	2934	2937	2941	rVB	766283	820717	5.60%	1.254%
30	20.522	2961	2964	2969	rVB2	711294	911112	6.22%	1.393%
31	20.674	2983	2990	2996	rBV2	1273989	2742218	18.71%	4.191%
32	20.816	3011	3014	3019	rVB	1793397	2102267	14.34%	3.213%
33	20.880	3022	3025	3028	rVV	736891	778833	5.31%	1.190%
34	21.080	3056	3059	3063	rVB	1625830	1745519	11.91%	2.668%
35	21.139	3066	3069	3073	rVB	905795	1042446	7.11%	1.593%
36	21.345	3100	3104	3105	rBV	1283209	1670450	11.40%	2.553%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010626.D
Acq On : 29 May 2022 19:10
Operator : CG/JU
Sample : N2928-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P026-SS001-1824-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.369	3105	3108	3114	rVB	3731453	4464397	30.46%	6.823%
38	21.474	3120	3126	3137	rBV	9302763	14656404	100.00%	22.400%
39	21.698	3160	3164	3169	rBV	1214567	1767046	12.06%	2.701%




Sum of corrected areas: 65429121

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010626.D
Acq On : 29 May 2022 19:10
Operator : CG/JU
Sample : N2928-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P026-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

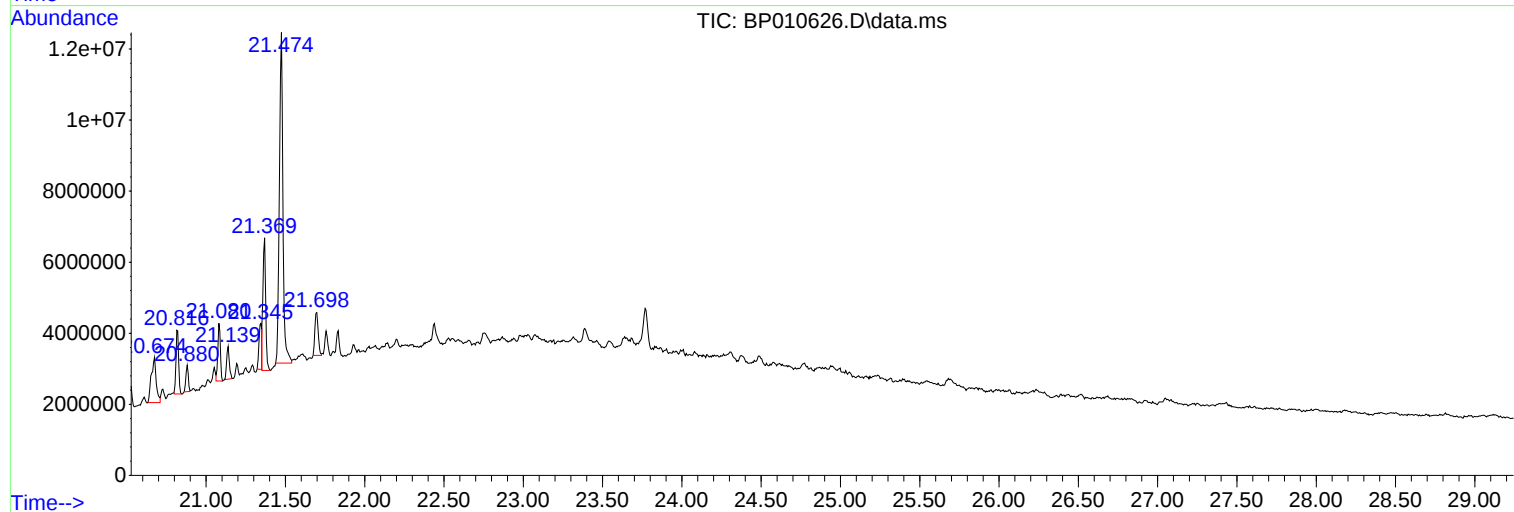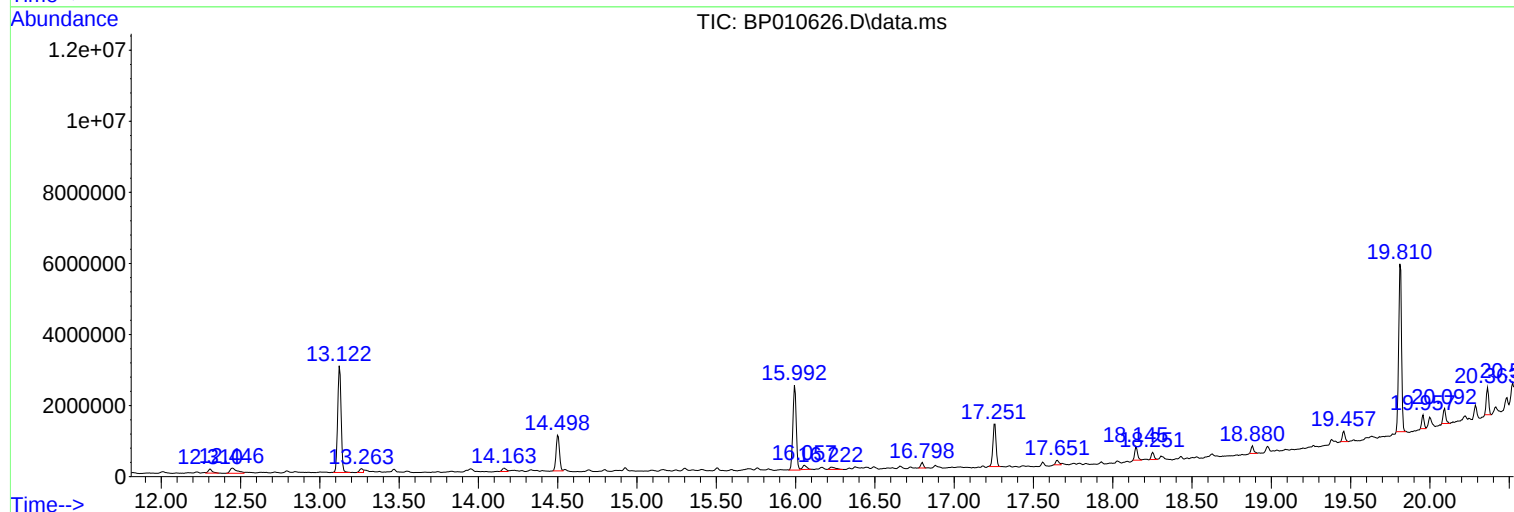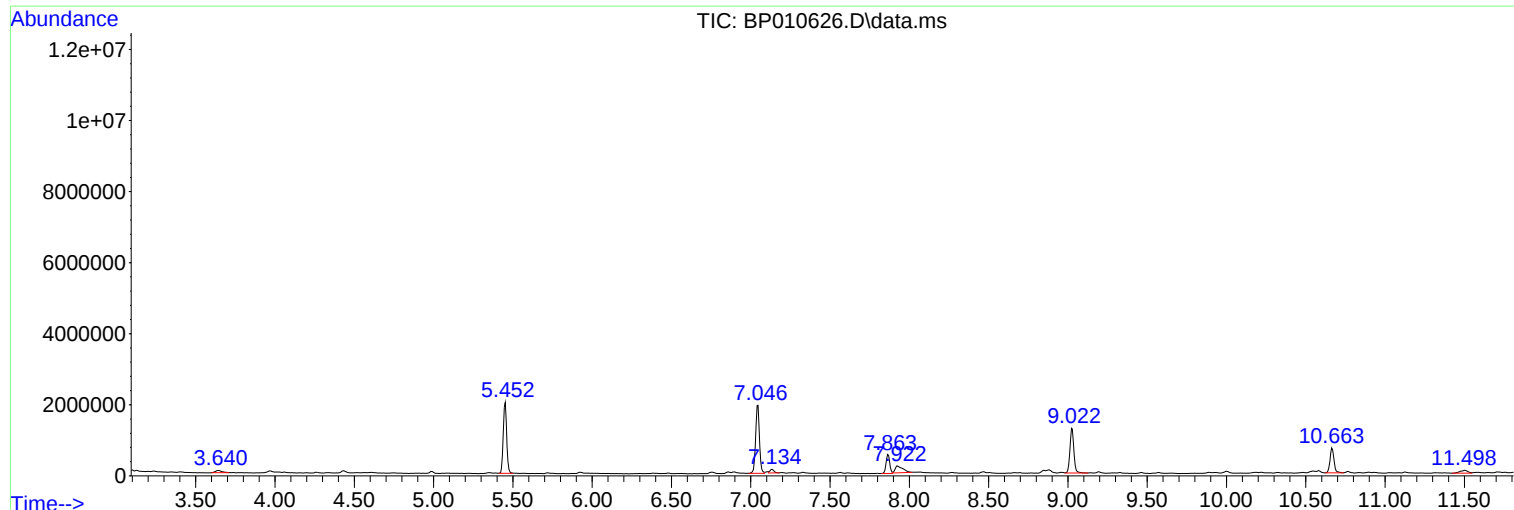

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010626.D
Acq On : 29 May 2022 19:10
Operator : CG/JU
Sample : N2928-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P026-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010626.D
Acq On : 29 May 2022 19:10
Operator : CG/JU
Sample : N2928-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
P026-SS001-1824-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------