


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
 Data File : BP010612.D
 Acq On : 29 May 2022 11:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 28 02:18:04 2022

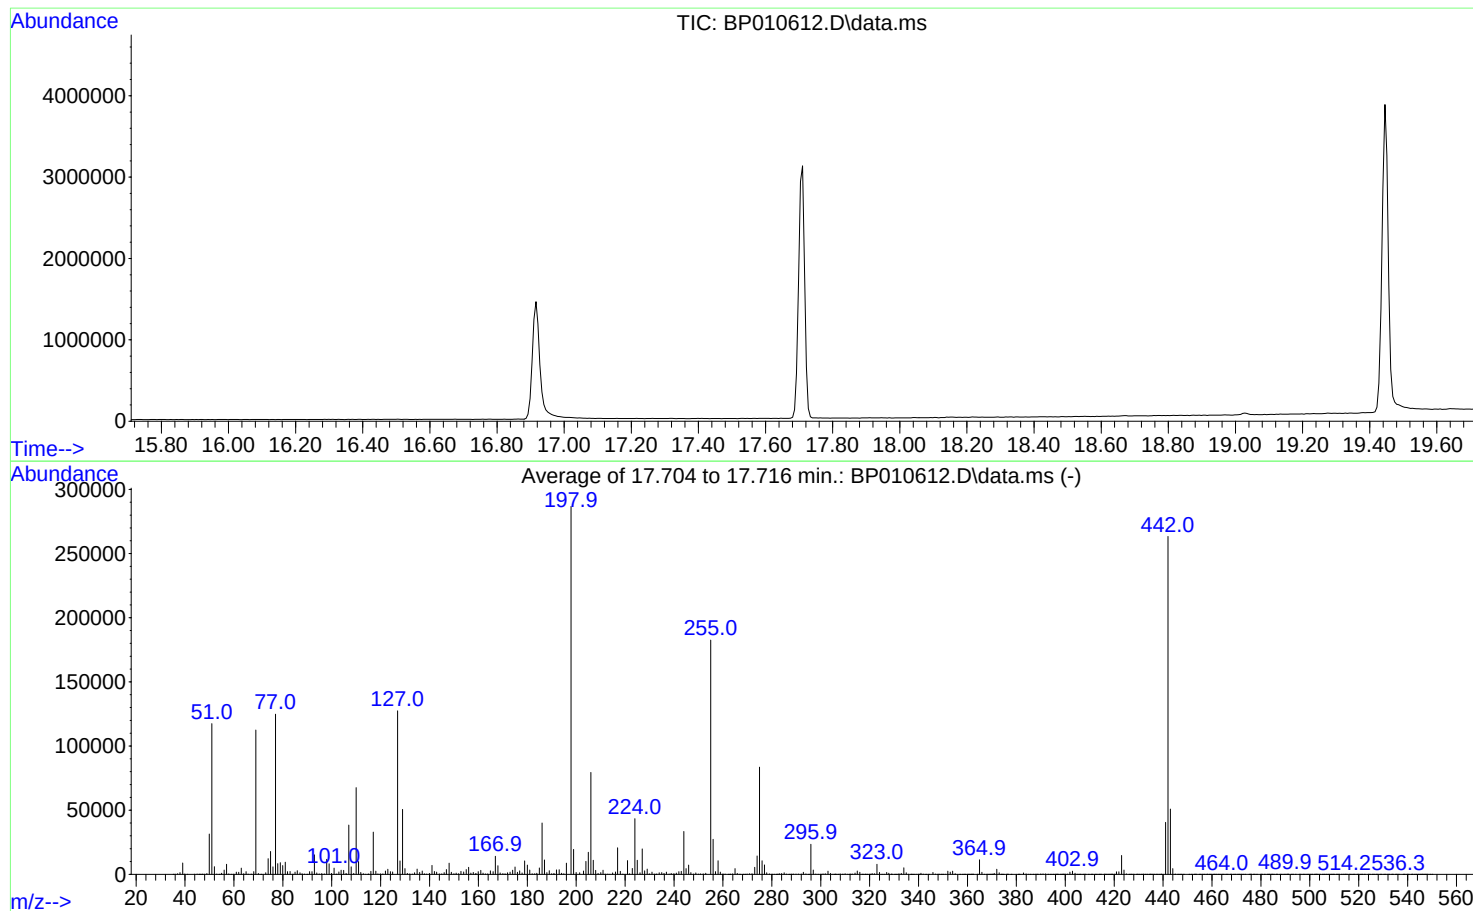




AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	117526	PASS
68	69	0.00	2	1.8	2079	PASS
69	198	0.00	100	39.2	112430	PASS
70	69	0.00	2	0.6	627	PASS
127	198	10	80	44.5	127458	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	286677	PASS
199	198	5	9	6.8	19412	PASS
275	198	10	60	29.1	83506	PASS
365	198	1	100	4.0	11391	PASS
441	198	0.01	100	14.1	40499	PASS
442	442	100	100	100.0	263317	PASS
443	442	15	24	19.3	50842	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
Data File : BP010612.D
Acq On : 29 May 2022 11:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 30 04:40:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

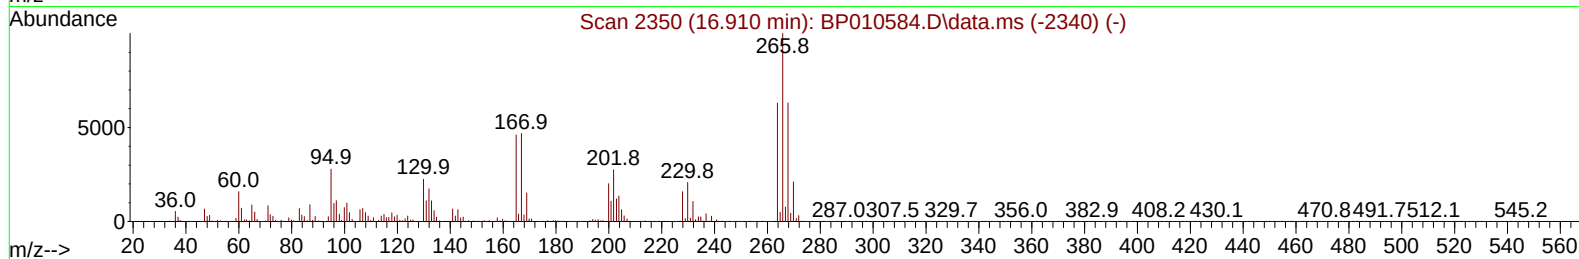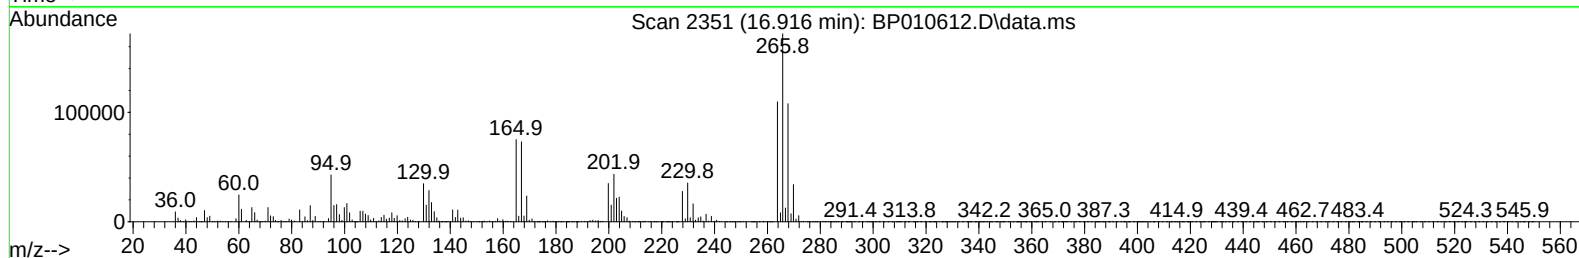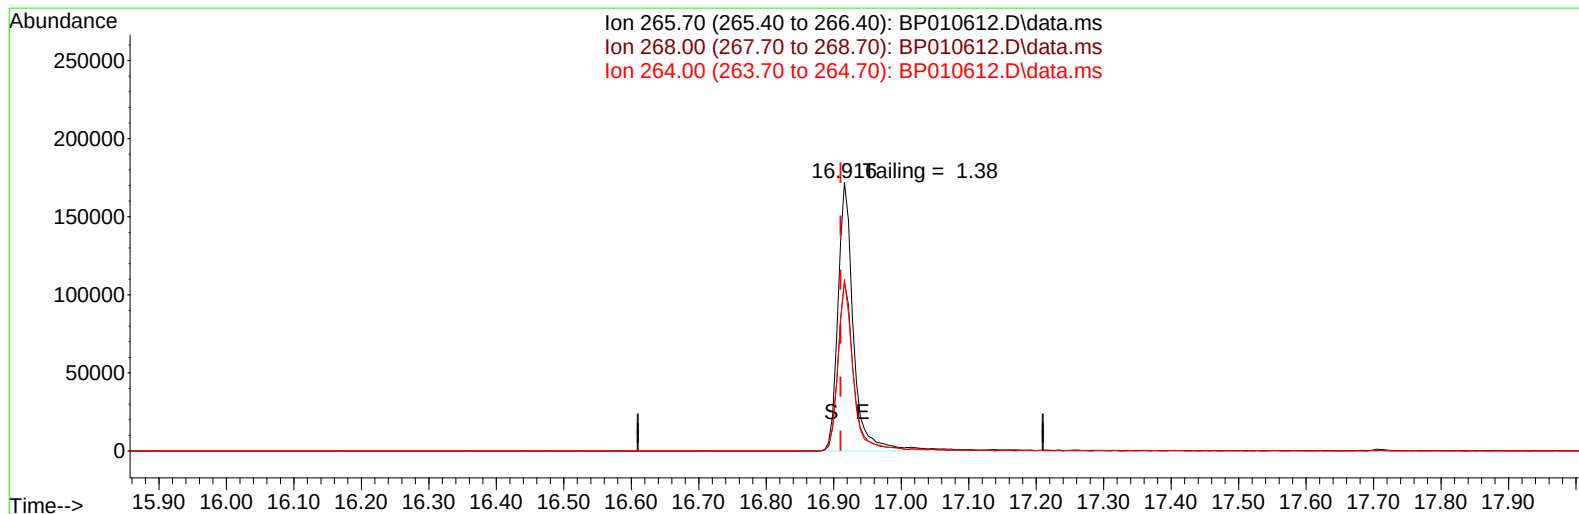

TIC: BP010612.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 341367.25 ng




response 270789

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.80
264.00	63.00	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052922\
 Data File : BP010612.D
 Acq On : 29 May 2022 11:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 30 04:40:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

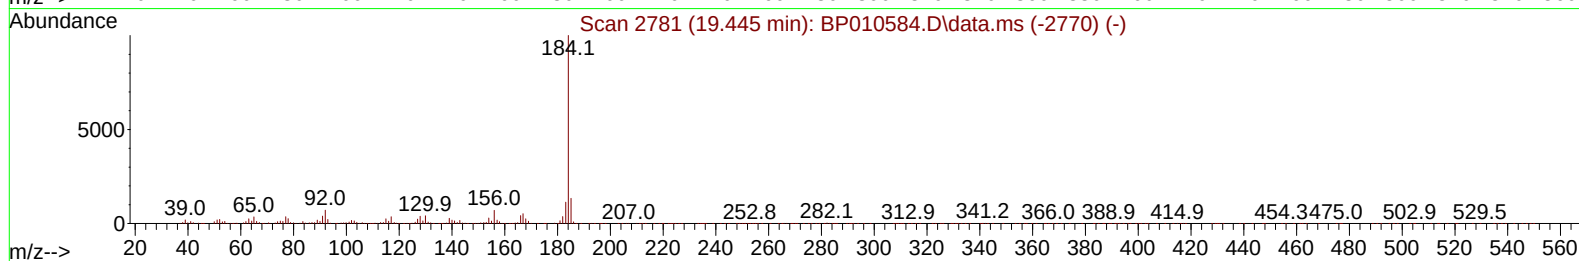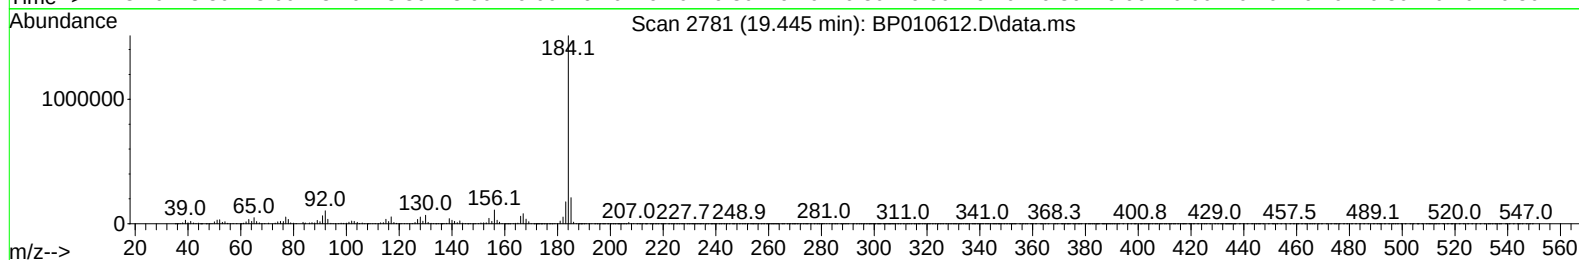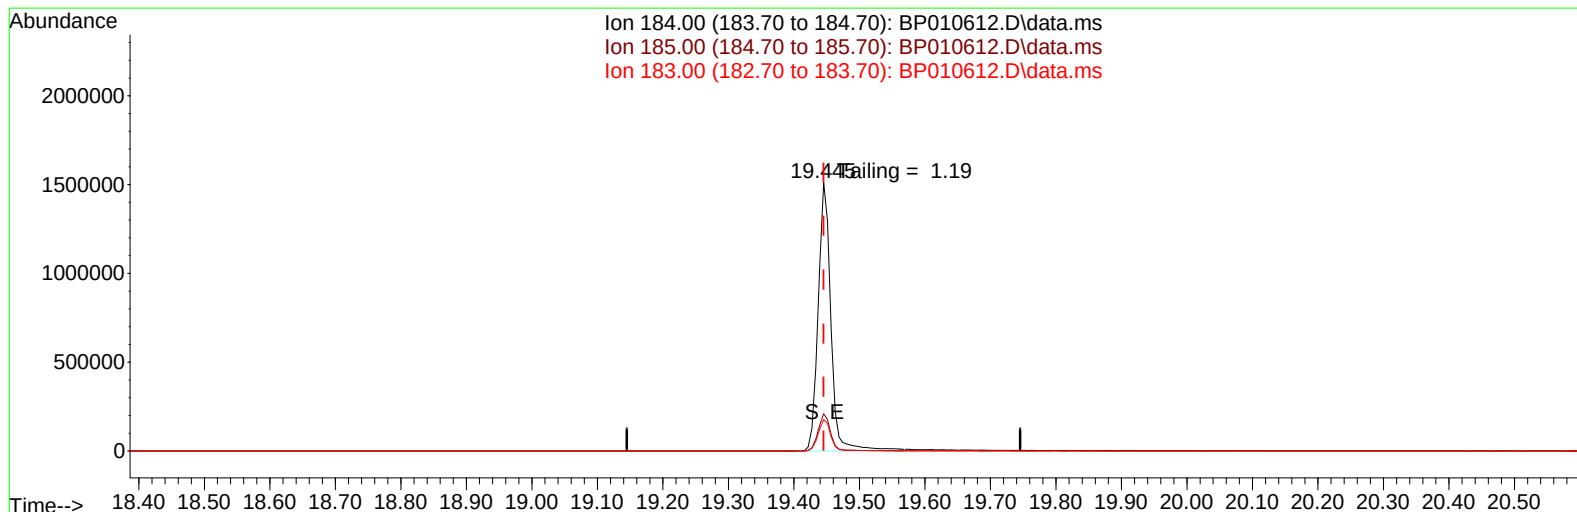

TIC: BP010612.D\data.ms

(77) Benzidine

19.445min (-0.000) 148180.42 ng

response 2060830

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.89
183.00	11.30	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/29/2022	BNA_P	<u>BP010612.D</u>
Compound Name	Response	Retention Time
DDT	1029309	20.651
DDD	13580	20.222
DDE	2184	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15764	1045073	1.51

Instrument :
BNA_P
ClientSampleId :
DFTPP