
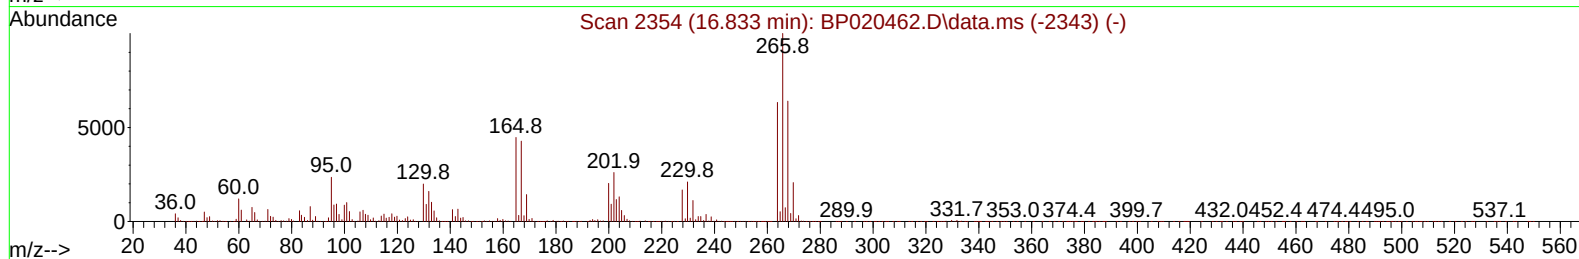
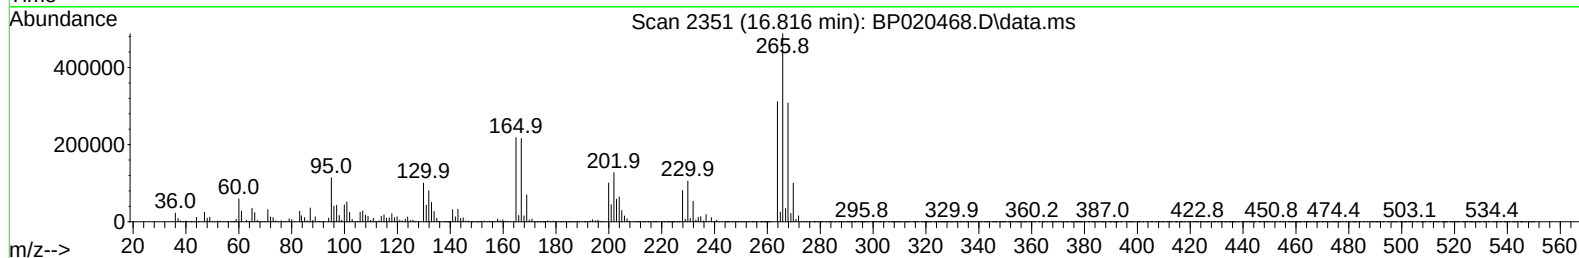


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052924\
Data File : BP020468.D
Acq On : 29 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 12:36:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 01:36:38 2024
Response via : Initial Calibration

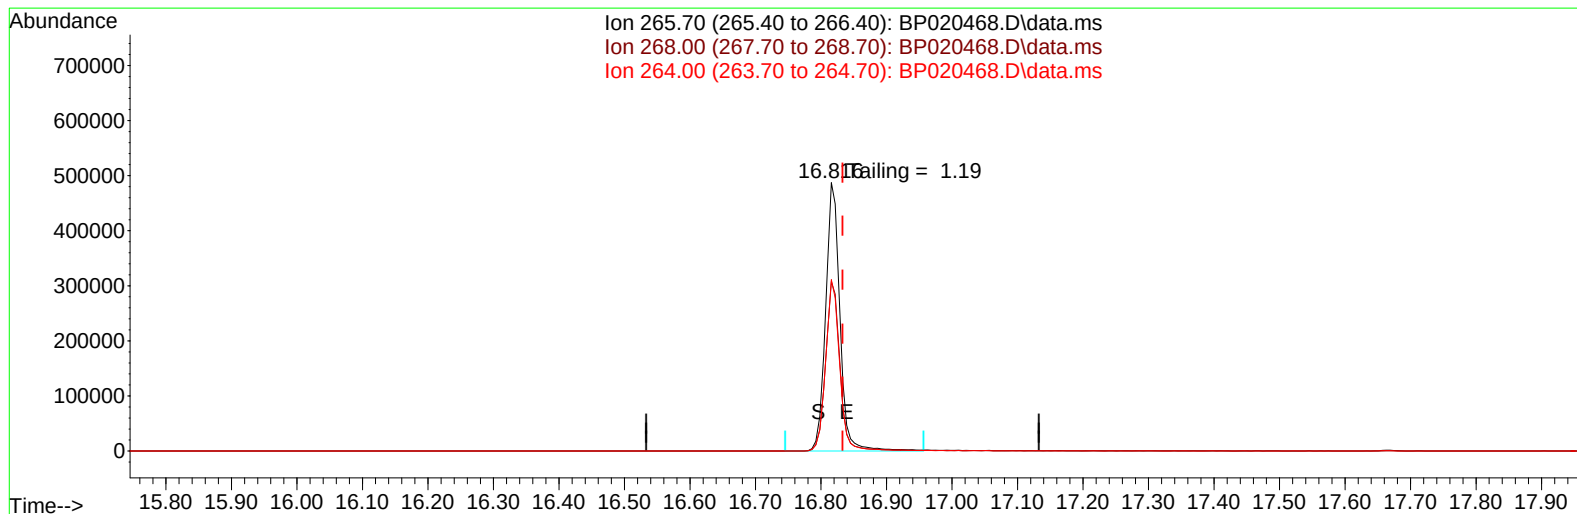

TIC: BP020468.D\data.ms

(70) Pentachlorophenol (C)




16.816min (-0.017) 245244.77 ng

response 740400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.13
264.00	63.30	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052924\
Data File : BP020468.D
Acq On : 29 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 12:36:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 01:36:38 2024
Response via : Initial Calibration

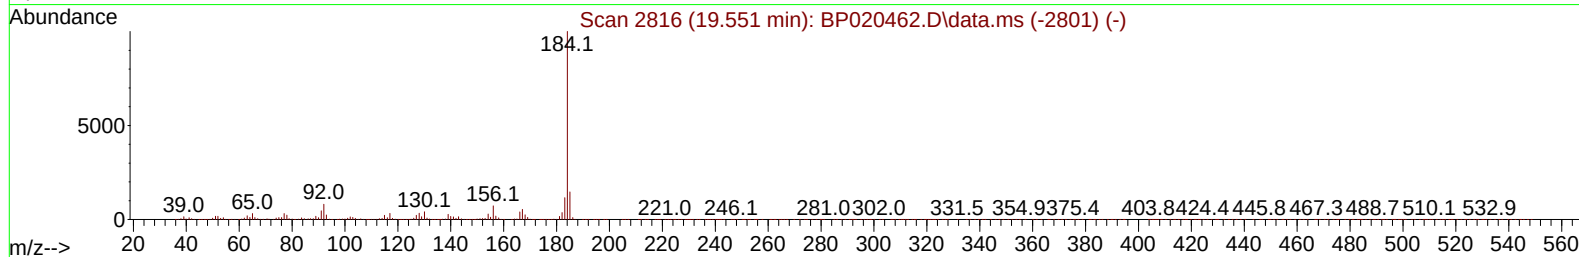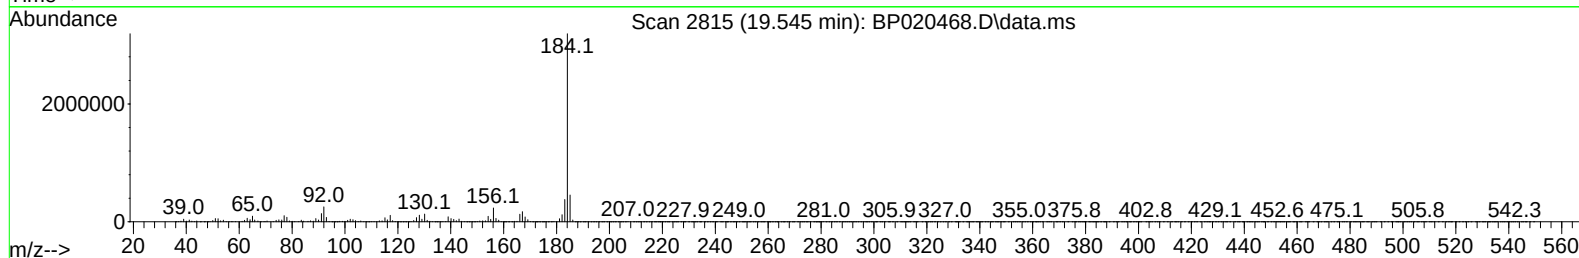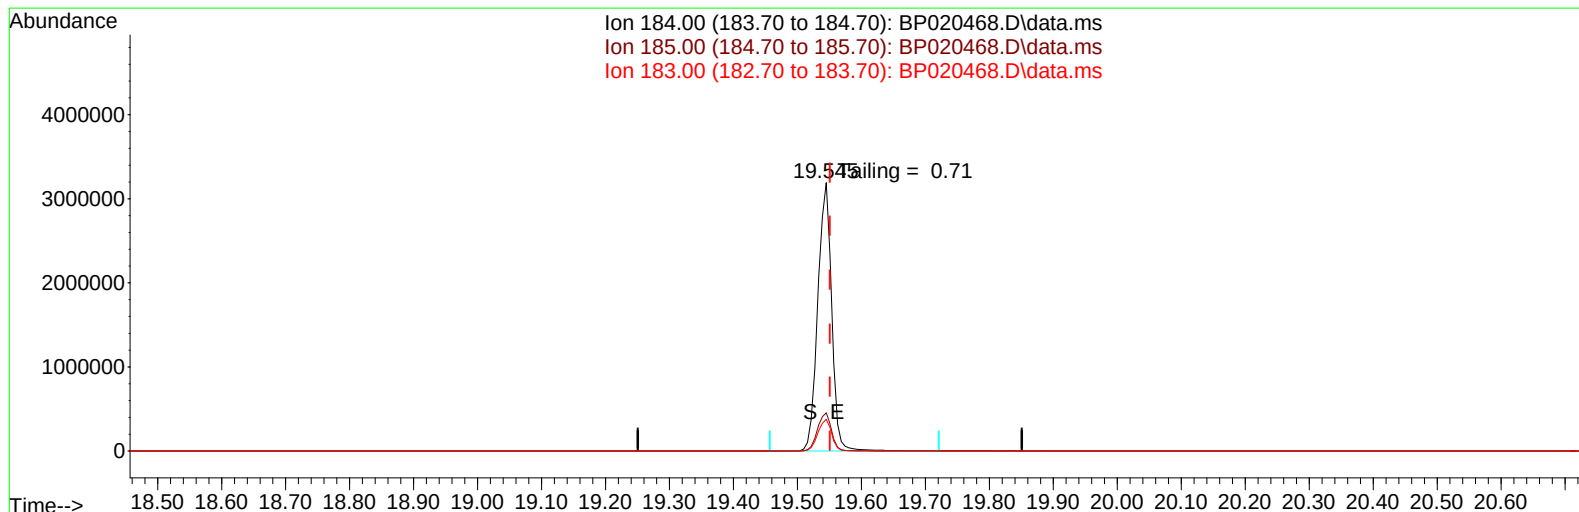

TIC: BP020468.D\data.ms

(77) Benzidine**19.545min (-0.006) 49713.48 ng****response 4828233**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	11.60	11.84
0.00	0.00	0.00