


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052924\
Data File : BP020468.D
Acq On : 29 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

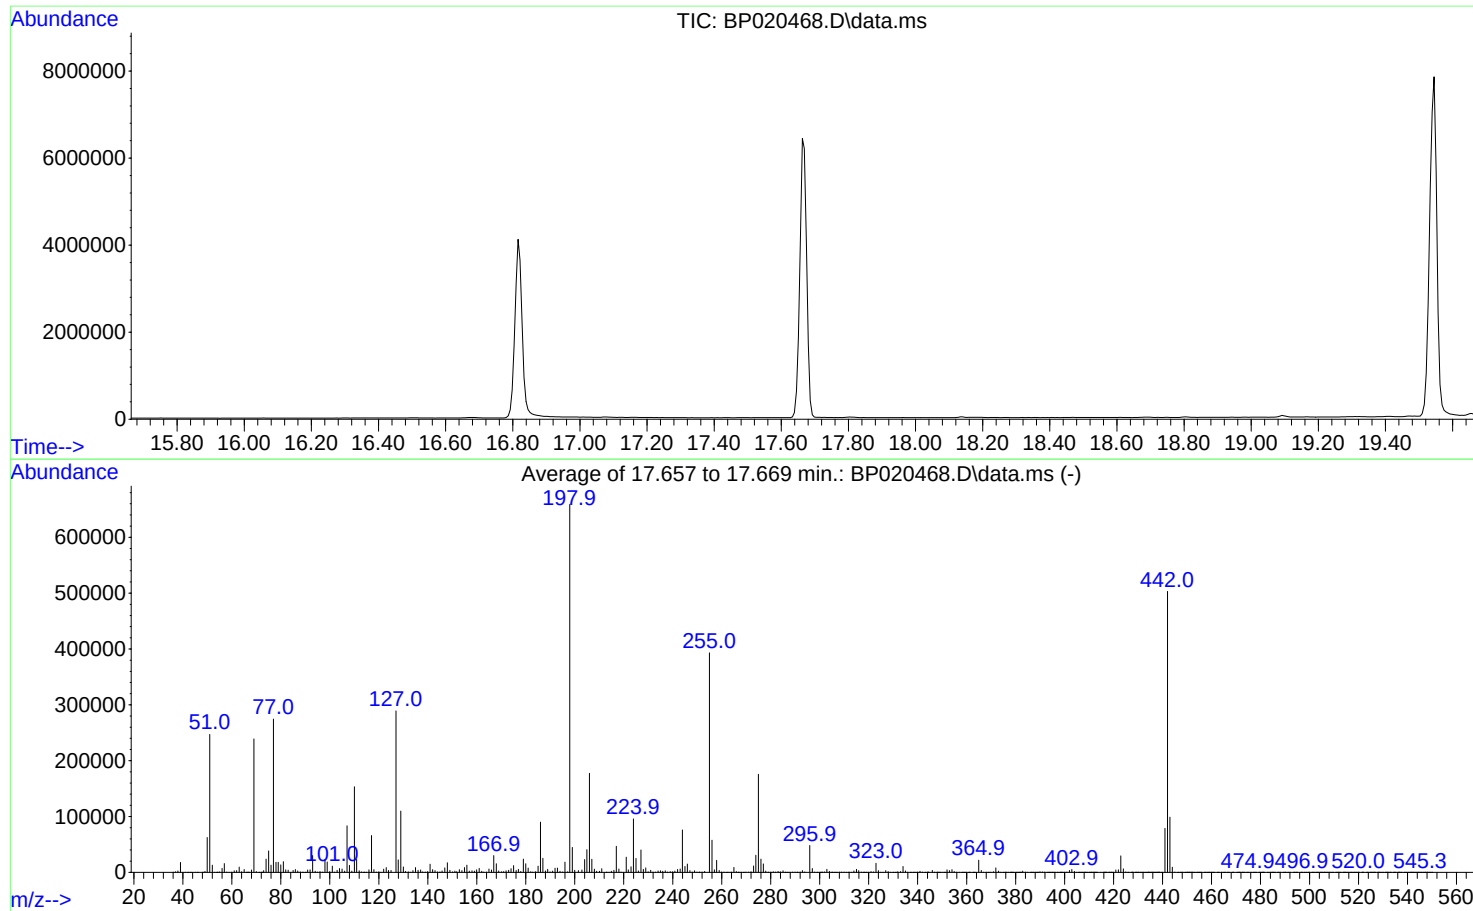




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	247101	PASS
68	69	0.00	2	1.8	4256	PASS
69	198	0.00	100	36.3	238882	PASS
70	69	0.00	2	0.6	1334	PASS
127	198	10	80	43.9	289146	PASS
197	198	0.00	2	0.2	1084	PASS
198	198	100	100	100.0	658731	PASS
199	198	5	9	6.8	44738	PASS
275	198	10	60	26.7	175624	PASS
365	198	1	100	3.3	21890	PASS
441	198	0.01	100	12.0	78779	PASS
442	442	100	100	100.0	503061	PASS
443	442	15	24	19.6	98744	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052924\
Data File : BP020468.D
Acq On : 29 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 29 12:36:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 01:36:38 2024
Response via : Initial Calibration

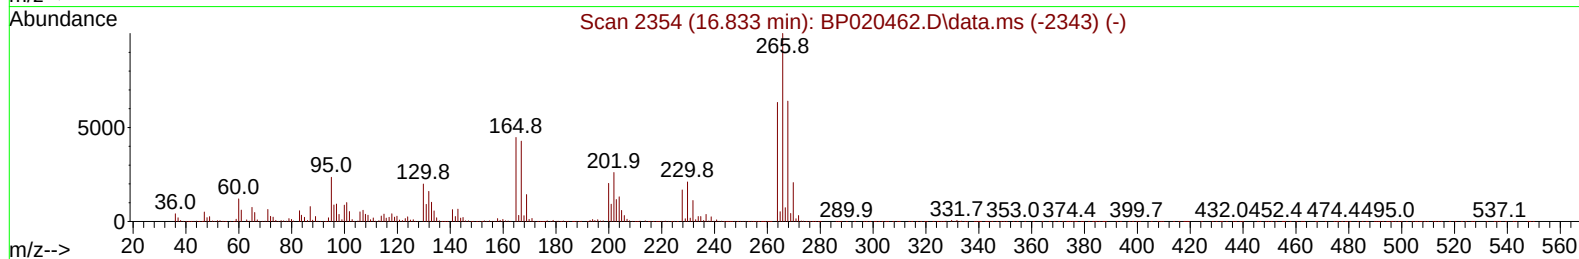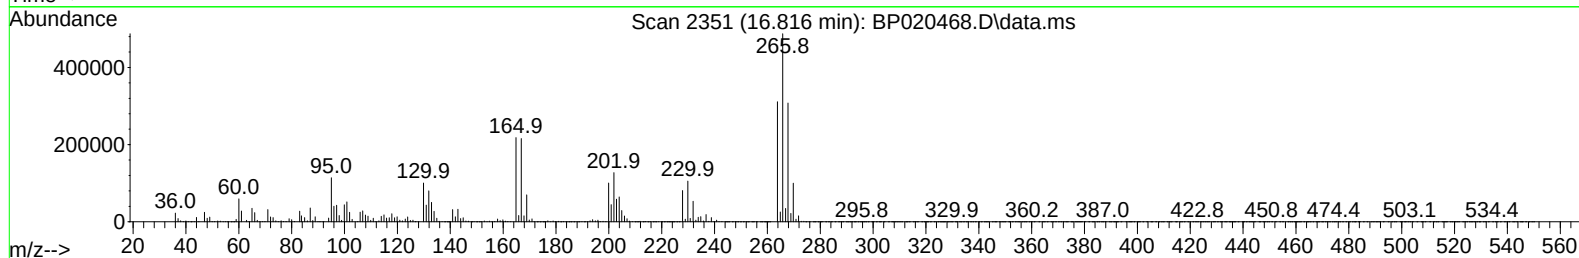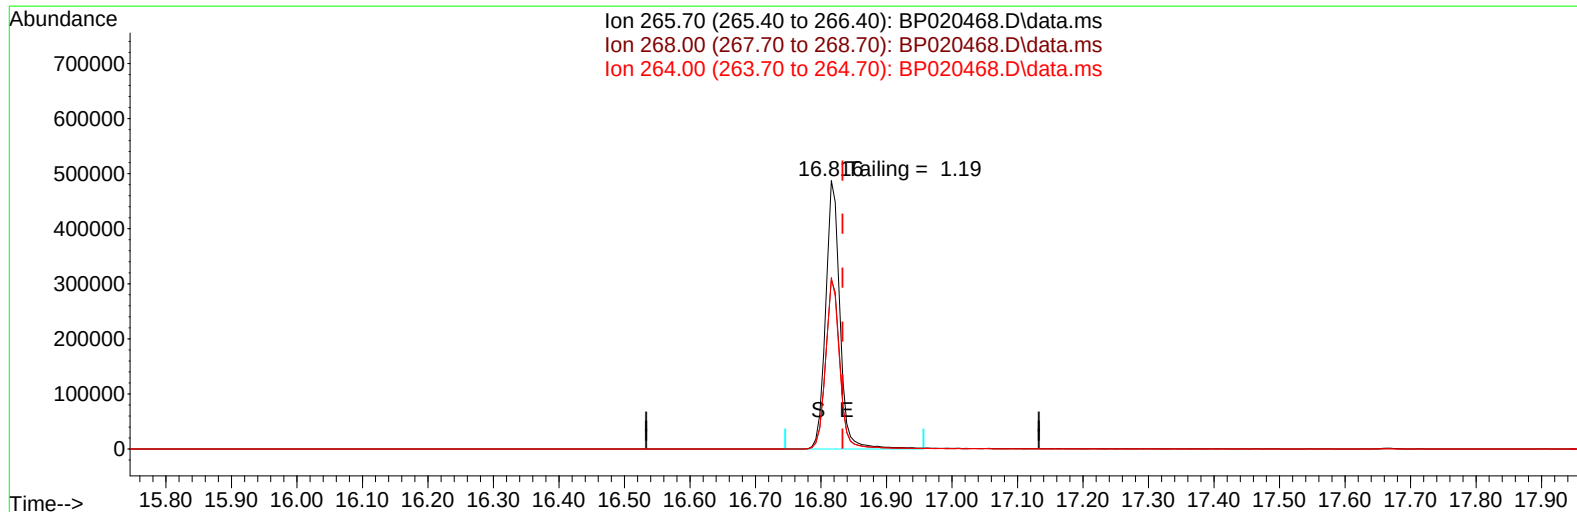

TIC: BP020468.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.017) 245244.77 ng




response 740400

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.13
264.00	63.30	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP052924\
Data File : BP020468.D
Acq On : 29 May 2024 09:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 29 12:36:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 29 01:36:38 2024
Response via : Initial Calibration

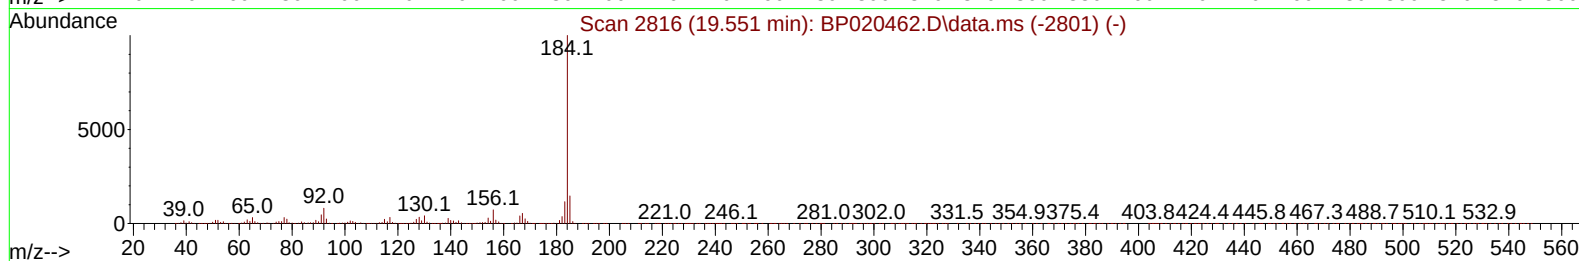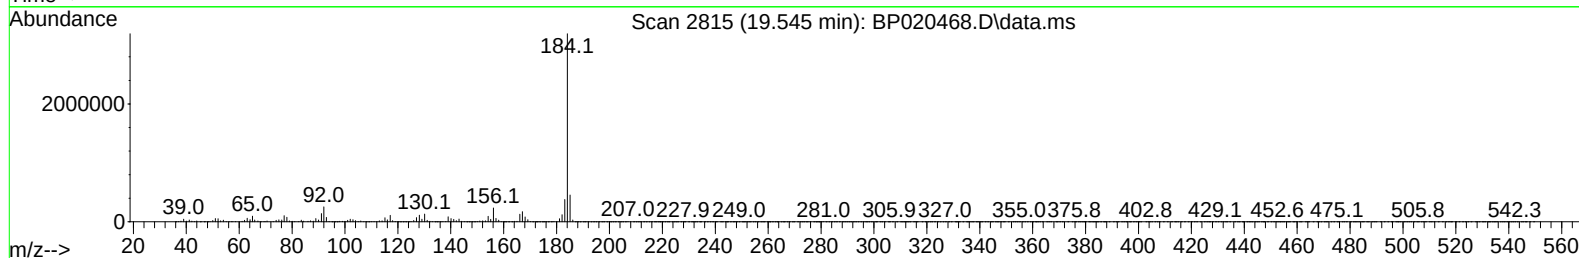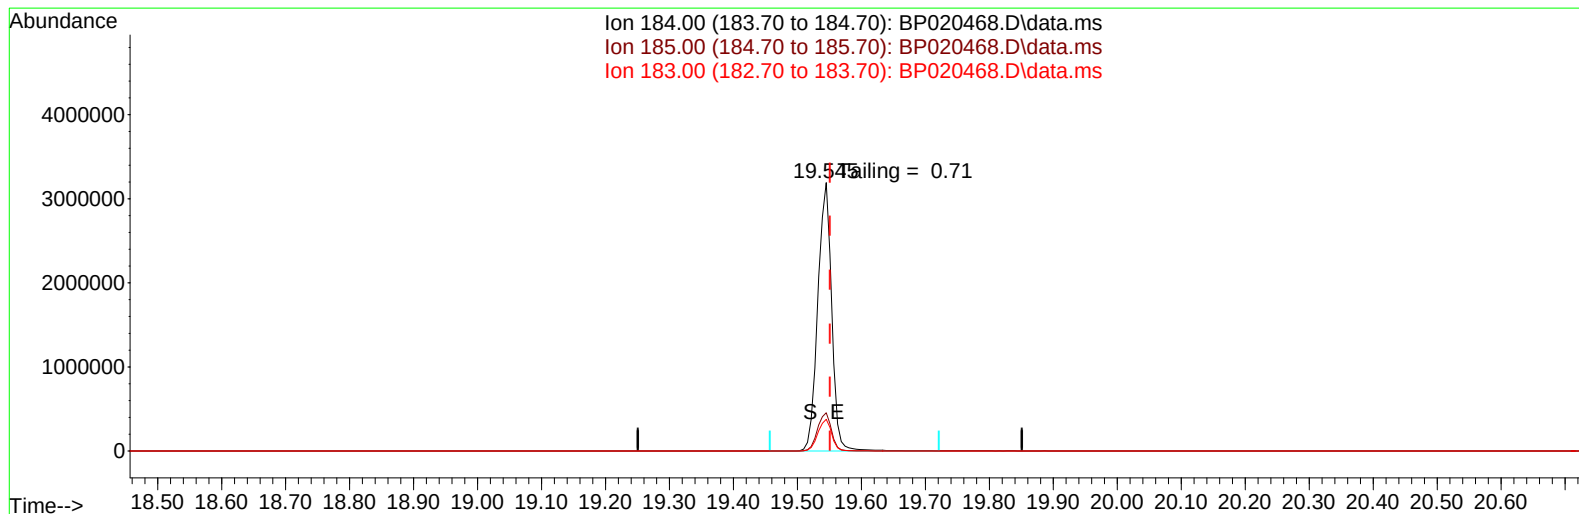

TIC: BP020468.D\data.ms

(77) Benzidine

19.545min (-0.006) 49713.48 ng

response 4828233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.24
183.00	11.60	11.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/29/2024	BNA_P	<u>BP020468.D</u>
Compound Name	Response	Retention Time
DDT	2195223	20.839
DDD	35135	20.374
DDE	2060	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37195	2232418	1.67

Instrument :
BNA_P
ClientSampleId :
DFTPP