
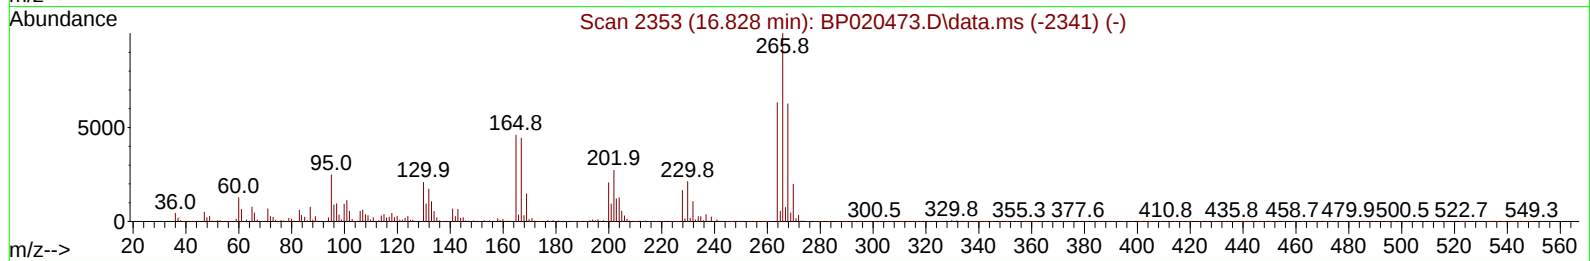
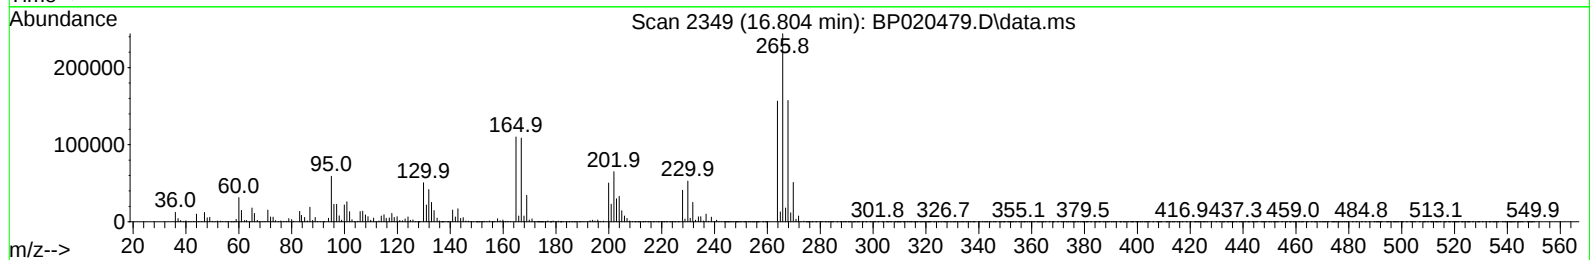


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP053024\  
Data File : BP020479.D  
Acq On : 30 May 2024 09:17  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 00:42:47 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 30 03:41:03 2024  
Response via : Initial Calibration

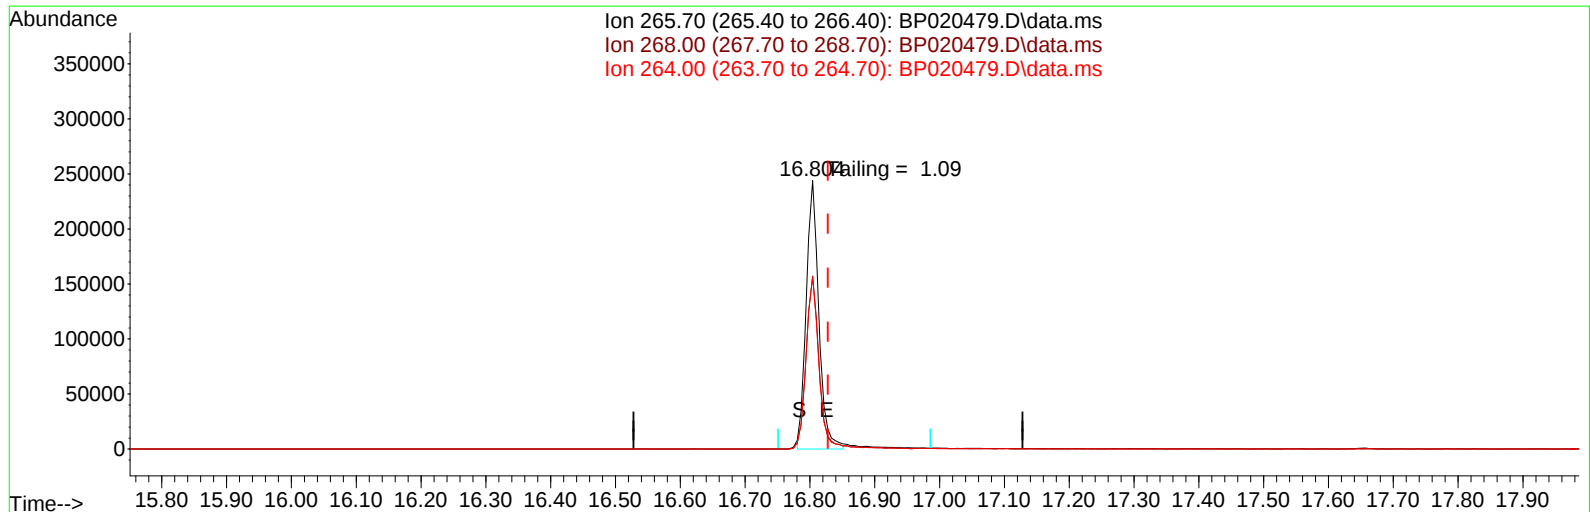

TIC: BP020479.D\data.ms

**(70) Pentachlorophenol (C)**




**16.804min (-0.024) 81495.13 ng**

**response 345057**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 64.47  |
| 264.00 | 63.30  | 64.16  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP053024\  
Data File : BP020479.D  
Acq On : 30 May 2024 09:17  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 00:42:47 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP052924.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu May 30 03:41:03 2024  
Response via : Initial Calibration

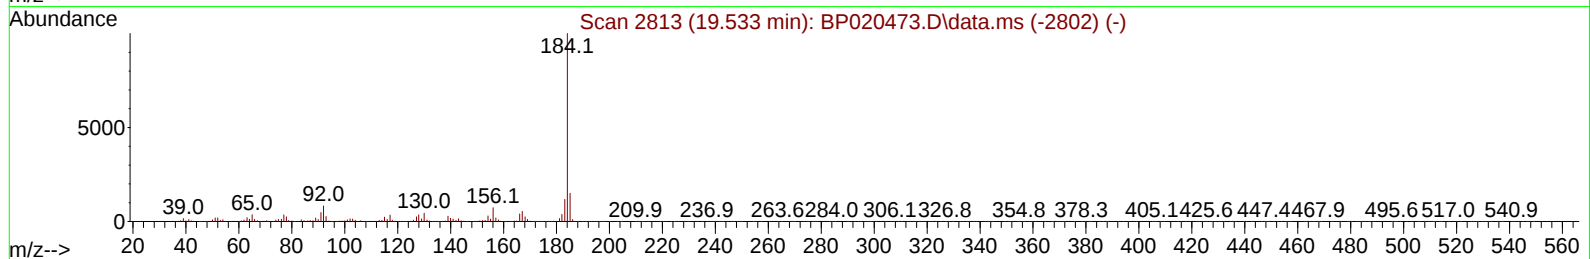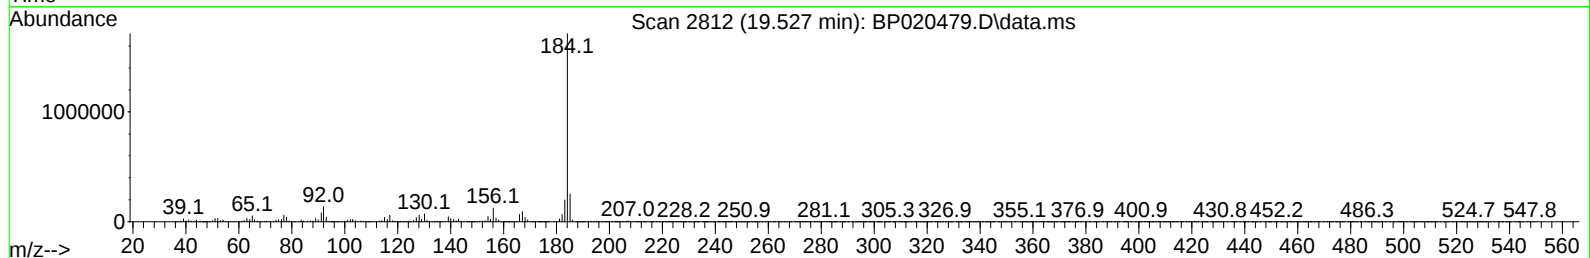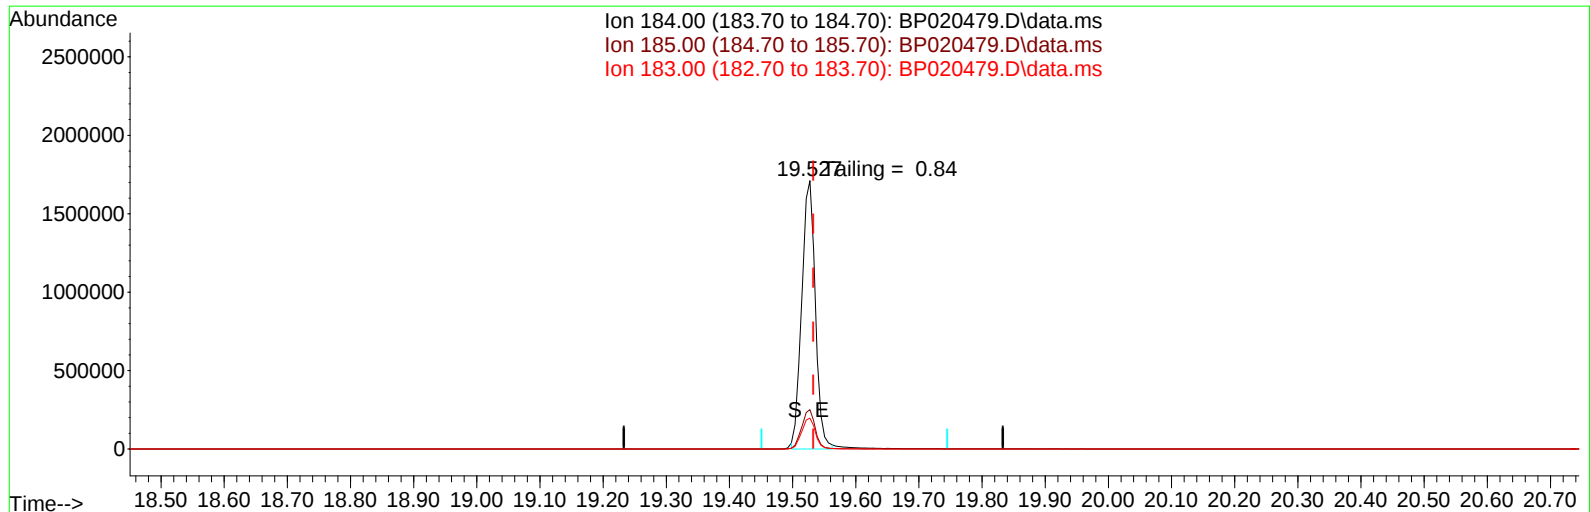

TIC: BP020479.D\data.ms

**(77) Benzidine****19.527min (-0.006) 11501.69 ng****response 2635292**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.70  |
| 183.00 | 11.70  | 11.54  |
| 0.00   | 0.00   | 0.00   |