
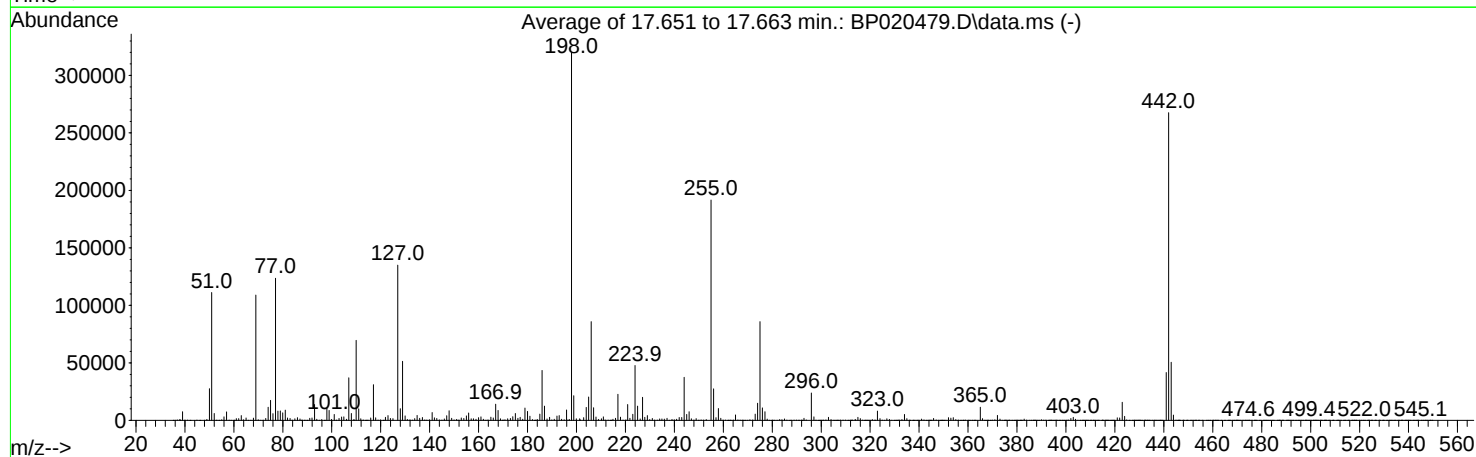


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053024\
Data File : BP020479.D
Acq On : 30 May 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 30 03:41:03 2024

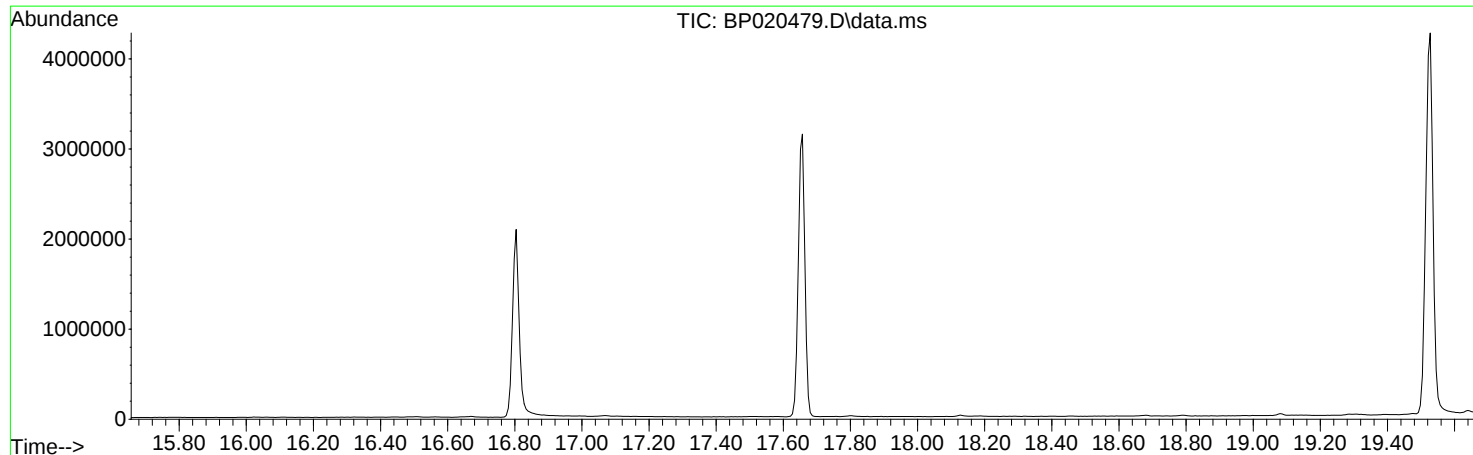




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	111152	PASS
68	69	0.00	2	1.8	1999	PASS
69	198	0.00	100	34.0	108928	PASS
70	69	0.00	2	0.5	532	PASS
127	198	10	80	42.2	134997	PASS
197	198	0.00	2	0.2	779	PASS
198	198	100	100	100.0	319936	PASS
199	198	5	9	6.7	21377	PASS
275	198	10	60	26.8	85888	PASS
365	198	1	100	3.6	11385	PASS
441	198	0.01	100	13.0	41667	PASS
442	442	100	100	100.0	267665	PASS
443	442	15	24	18.9	50475	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053024\
Data File : BP020479.D
Acq On : 30 May 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 31 00:42:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

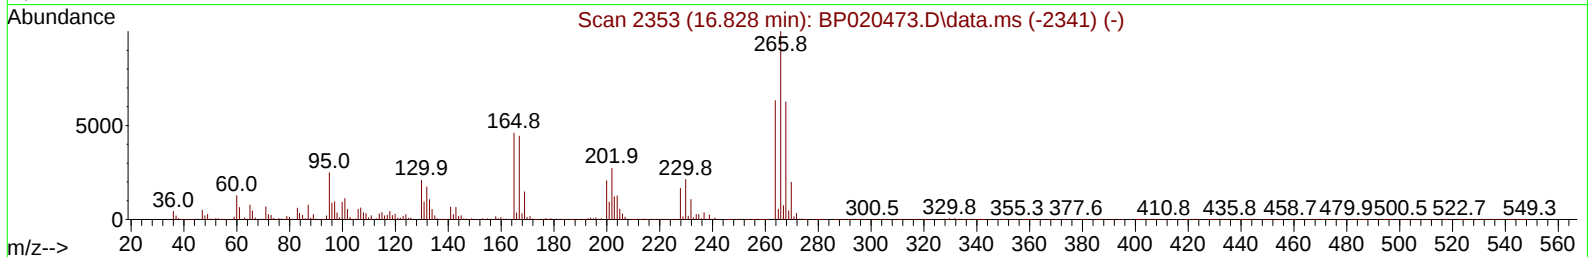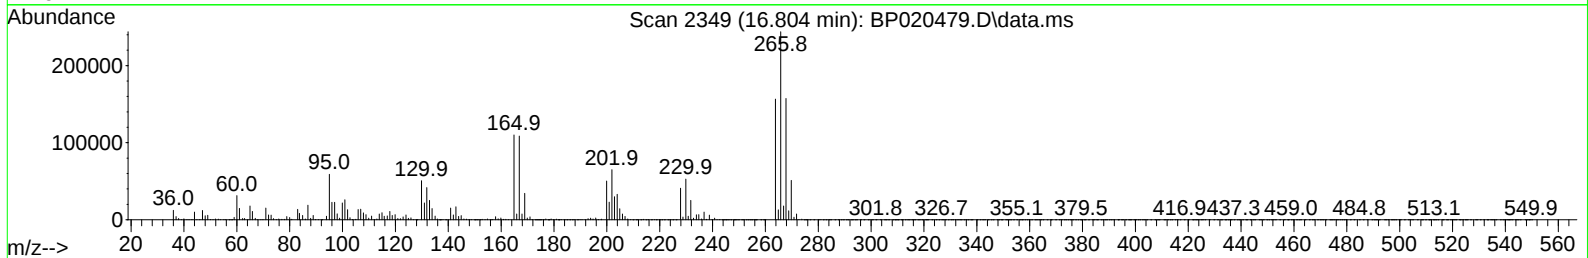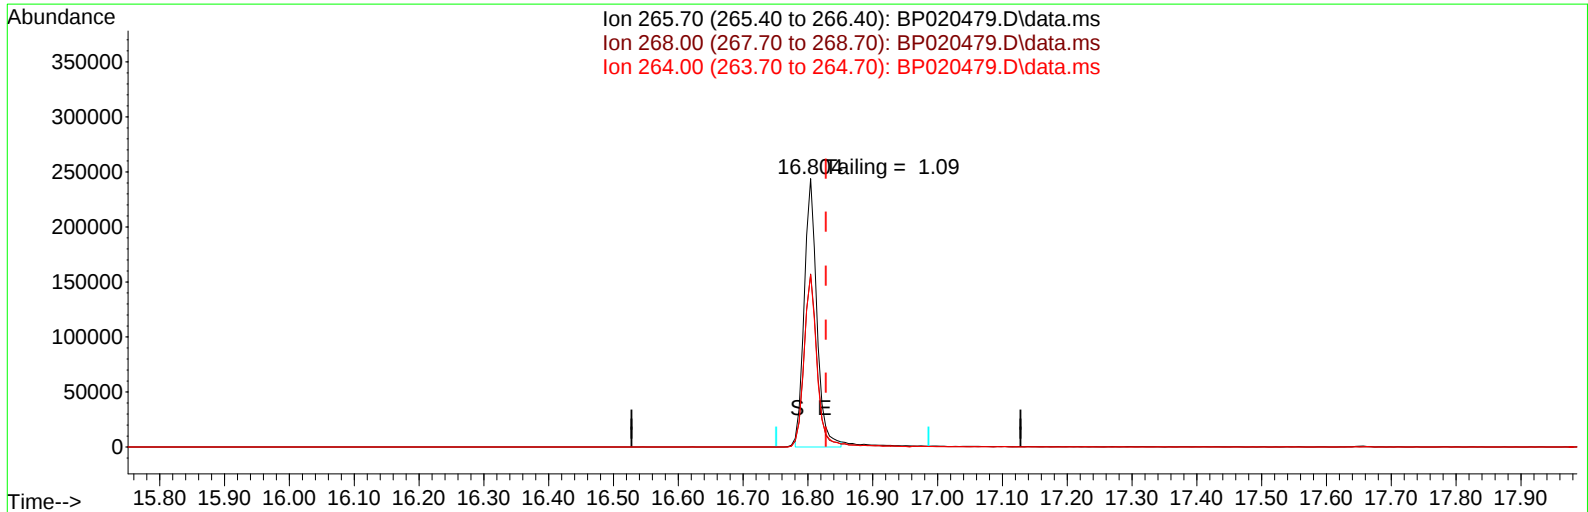

TIC: BP020479.D\data.ms

(70) Pentachlorophenol (C)

16.804min (-0.024) 81495.13 ng




response 345057

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.47
264.00	63.30	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053024\
Data File : BP020479.D
Acq On : 30 May 2024 09:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: May 31 00:42:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 30 03:41:03 2024
Response via : Initial Calibration

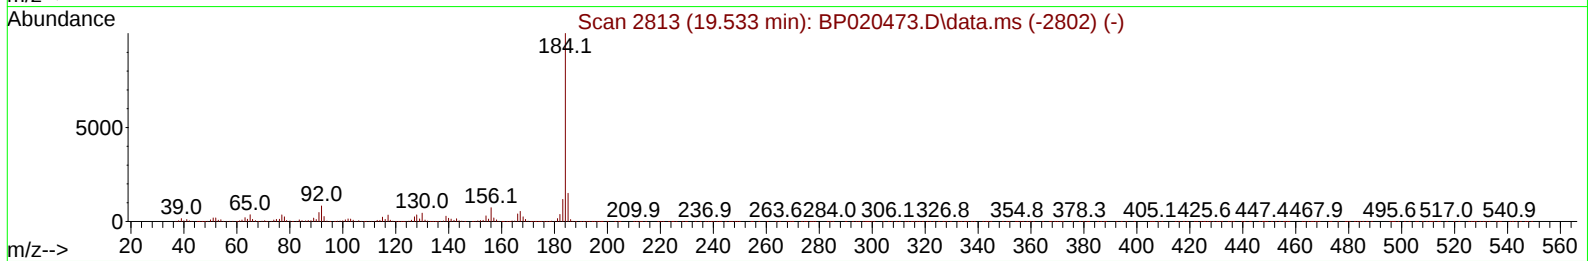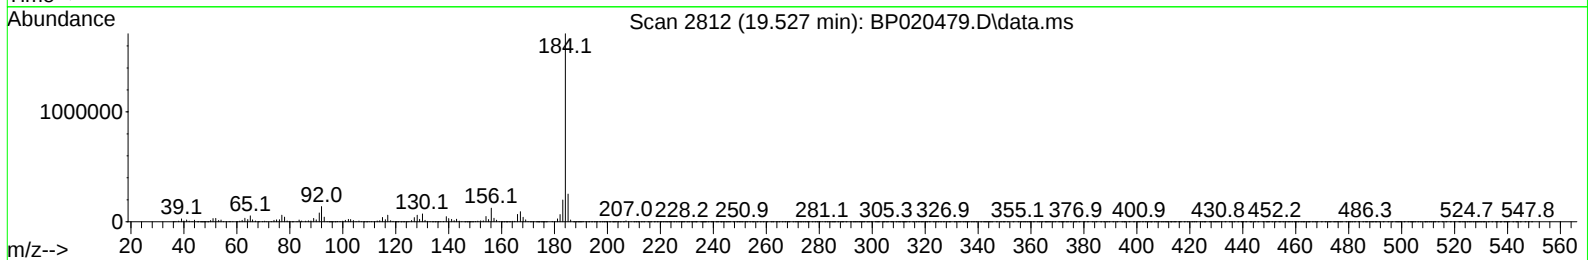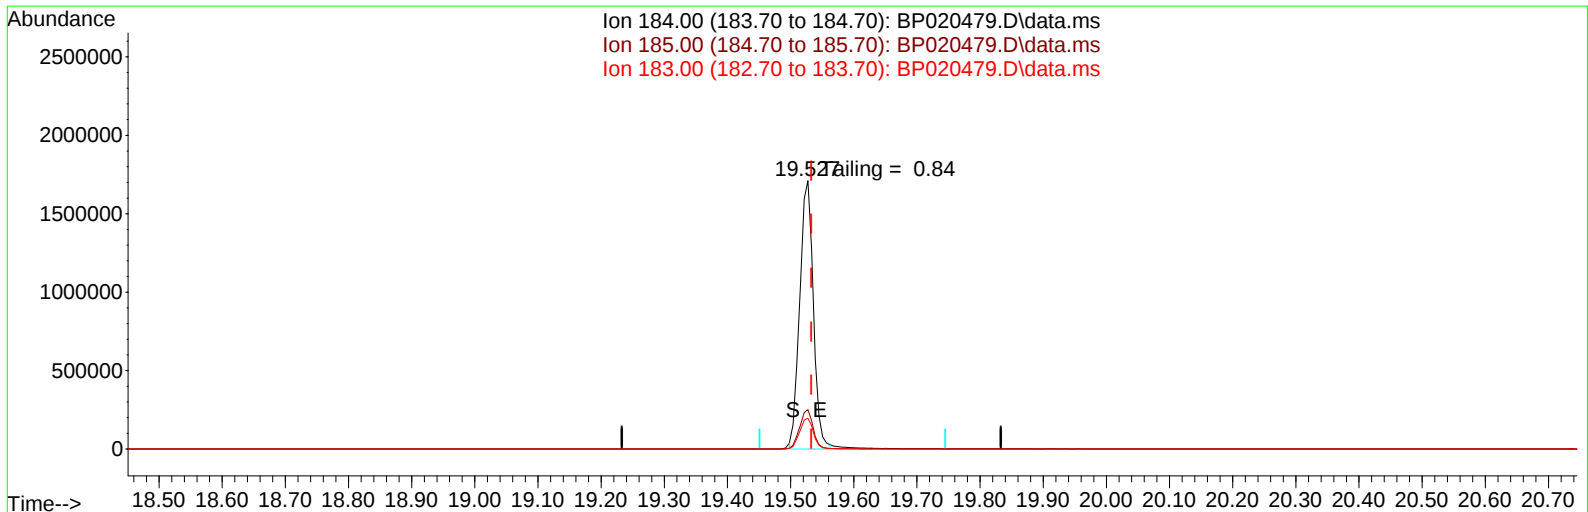

TIC: BP020479.D\data.ms

(77) Benzidine

19.527min (-0.006) 11501.69 ng

response 2635292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.70
183.00	11.70	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/30/2024	BNA_P	<u>BP020479.D</u>
Compound Name	Response	Retention Time
DDT	1022847	20.827
DDD	11617	20.416
DDE	668	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12285	1035132	1.19

Instrument :
BNA_P
ClientSampleId :
DFTPP