
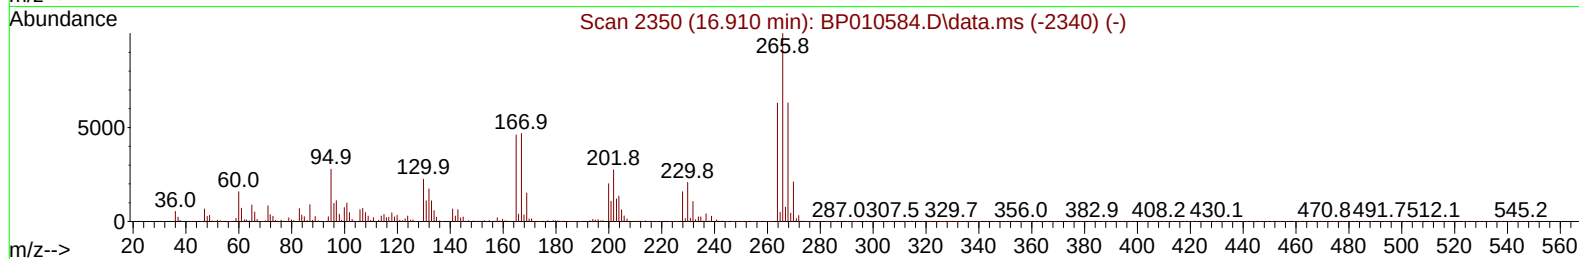
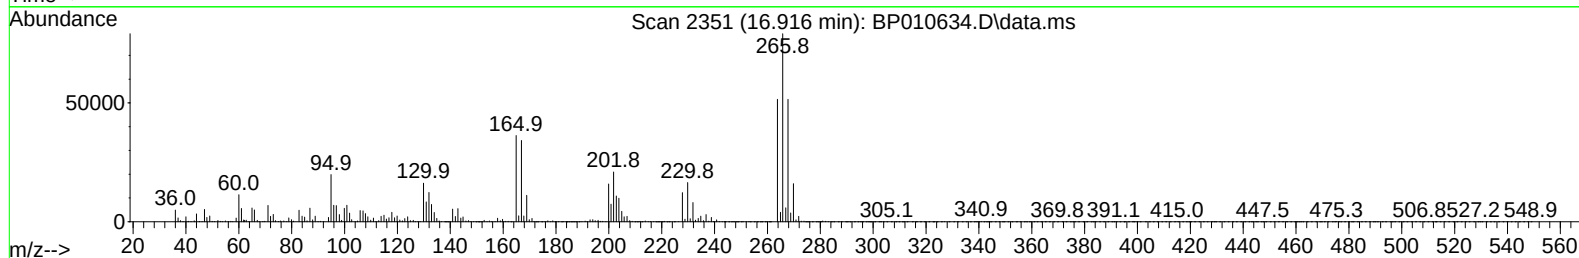


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
 Data File : BP010634.D
 Acq On : 31 May 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 06:03:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

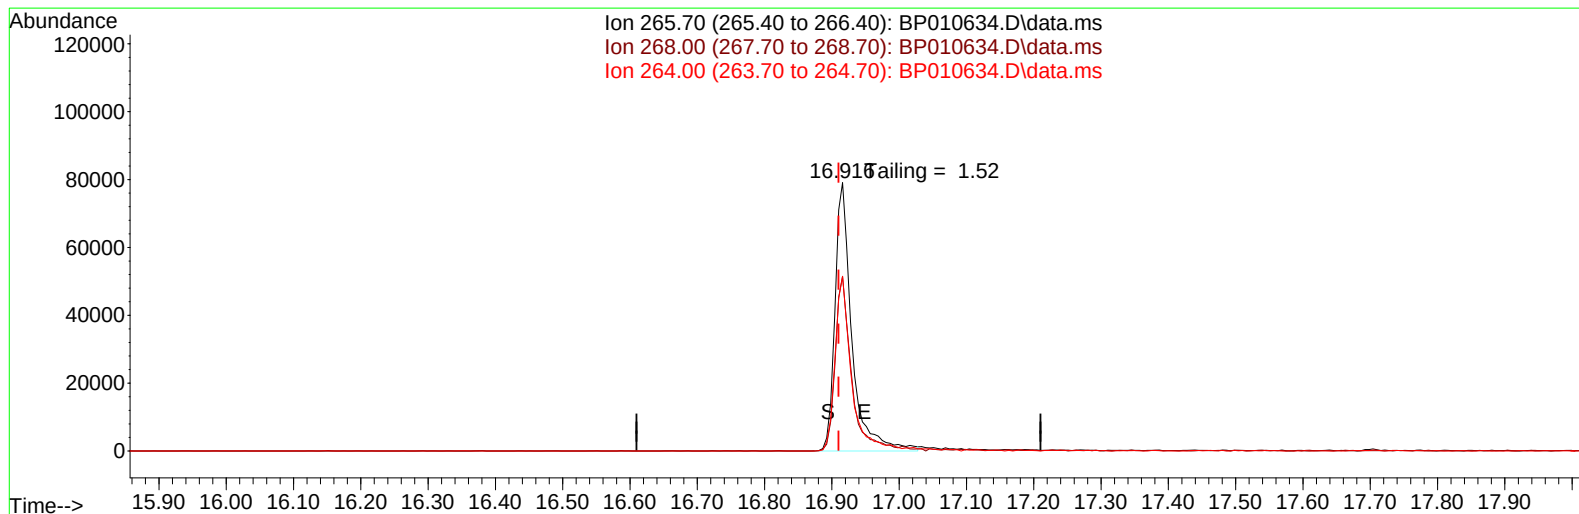

TIC: BP010634.D\data.ms

(70) Pentachlorophenol (C)




16.916min (+ 0.006) 2838105.14 ng

response 137037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.11
264.00	63.00	65.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
 Data File : BP010634.D
 Acq On : 31 May 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 06:03:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 28 02:18:04 2022
 Response via : Initial Calibration

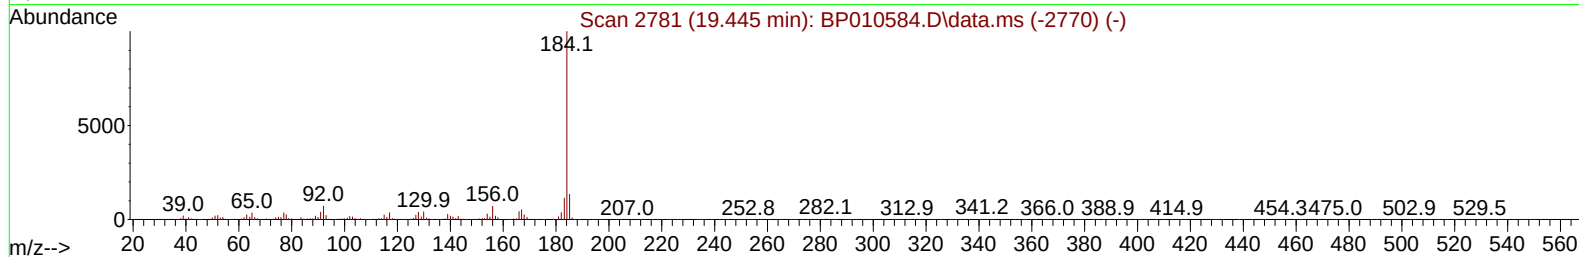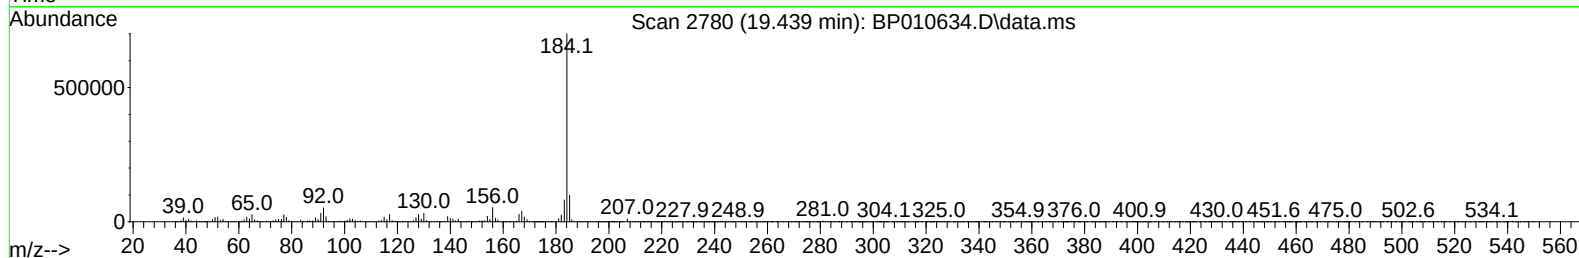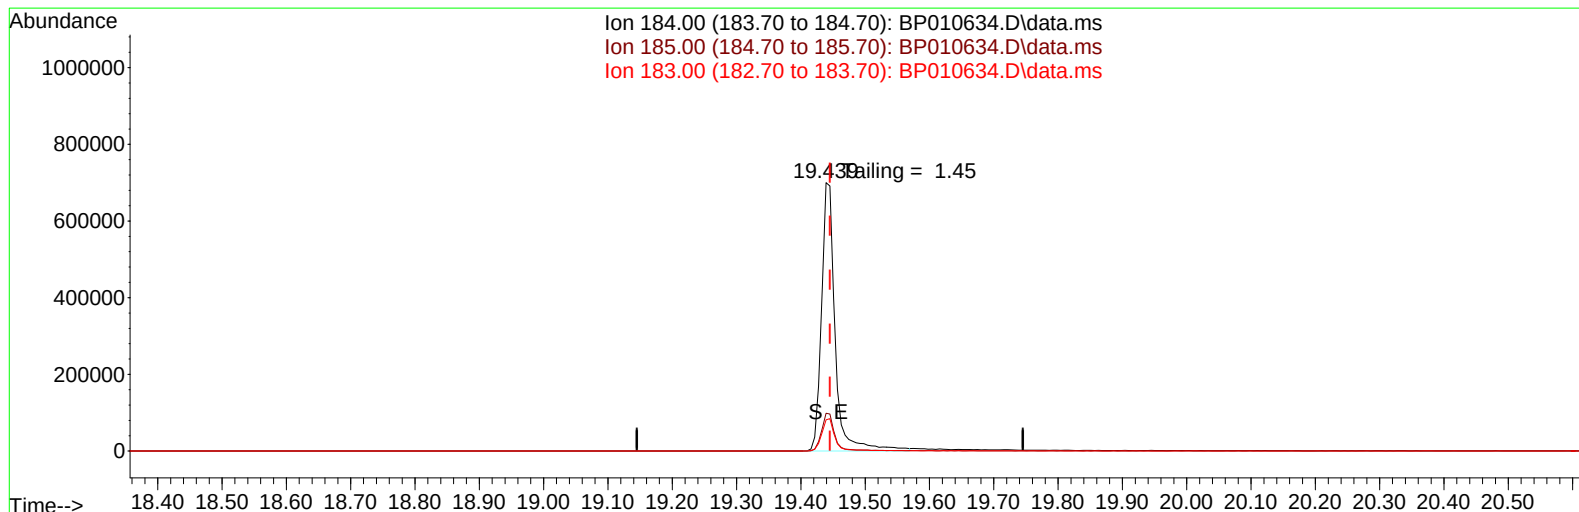

TIC: BP010634.D\data.ms

(77) Benzidine**19.439min (-0.006) 391319.02 ng****response 1052378**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.10
183.00	11.30	11.62
0.00	0.00	0.00