

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
 Data File : BP010636.D
 Acq On : 31 May 2022 13:03
 Operator : CG/JU
 Sample : PB145156BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB145156BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP010636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	395	402	417	rBV	2769121	4160280	55.57%	11.504%
2	7.040	665	672	688	rBV	2547799	4244729	56.70%	11.737%
3	7.863	805	812	825	rBV	502740	811250	10.84%	2.243%
4	9.028	1002	1010	1022	rBV	1568031	2764735	36.93%	7.645%
5	10.663	1280	1288	1303	rBV	569799	1060248	14.16%	2.932%
6	13.122	1698	1706	1730	rBV	3860161	5900299	78.81%	16.315%
7	14.498	1933	1940	1953	rBV	830290	1325740	17.71%	3.666%
8	15.998	2186	2195	2212	rBV	2673777	4287625	57.27%	11.856%
9	17.257	2402	2409	2426	rBV	947851	1465632	19.58%	4.053%
10	19.816	2838	2844	2855	rBV	5787071	7486480	100.00%	20.701%
11	21.339	3099	3103	3111	rBV	917133	1325599	17.71%	3.665%
12	23.757	3508	3514	3526	rVB2	606775	1332623	17.80%	3.685%




Sum of corrected areas: 36165240

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
Data File : BP010636.D
Acq On : 31 May 2022 13:03
Operator : CG/JU
Sample : PB145156BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145156BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

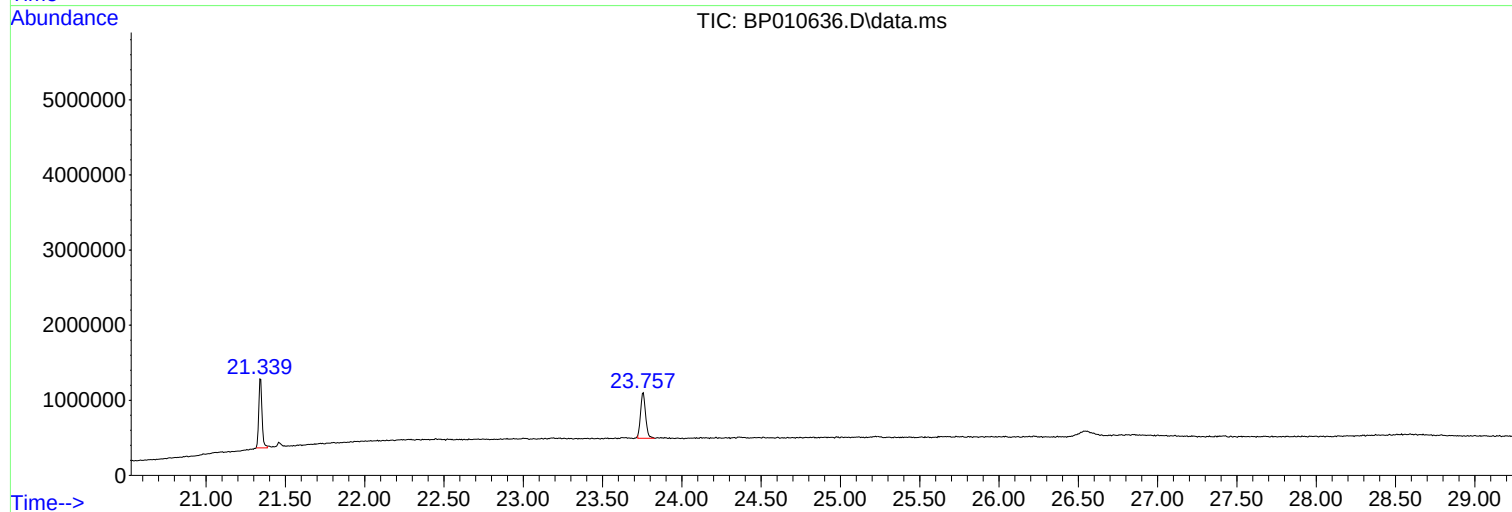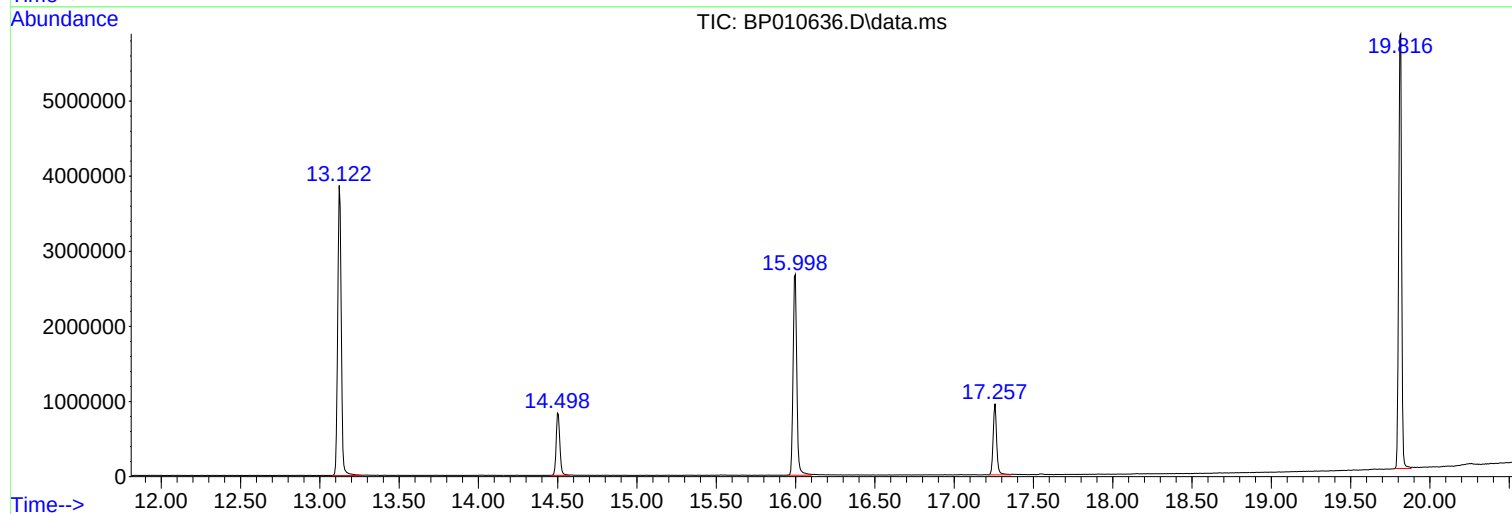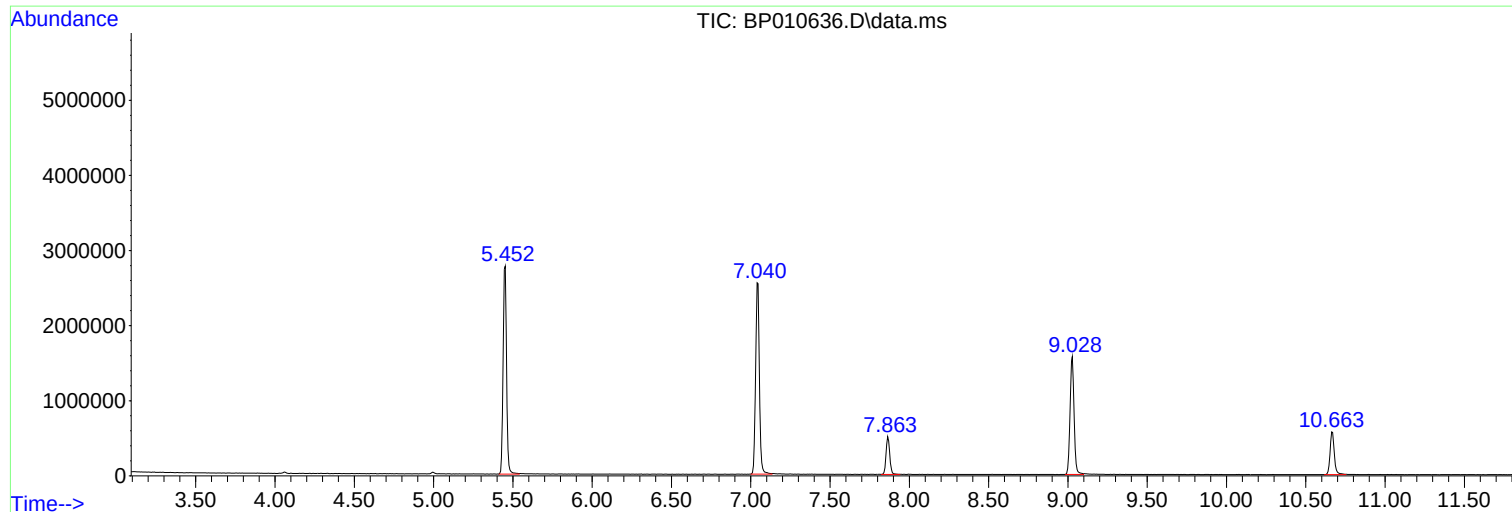

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
Data File : BP010636.D
Acq On : 31 May 2022 13:03
Operator : CG/JU
Sample : PB145156BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145156BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
Data File : BP010636.D
Acq On : 31 May 2022 13:03
Operator : CG/JU
Sample : PB145156BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB145156BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------