


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
 Data File : BP010634.D
 Acq On : 31 May 2022 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 28 02:18:04 2022

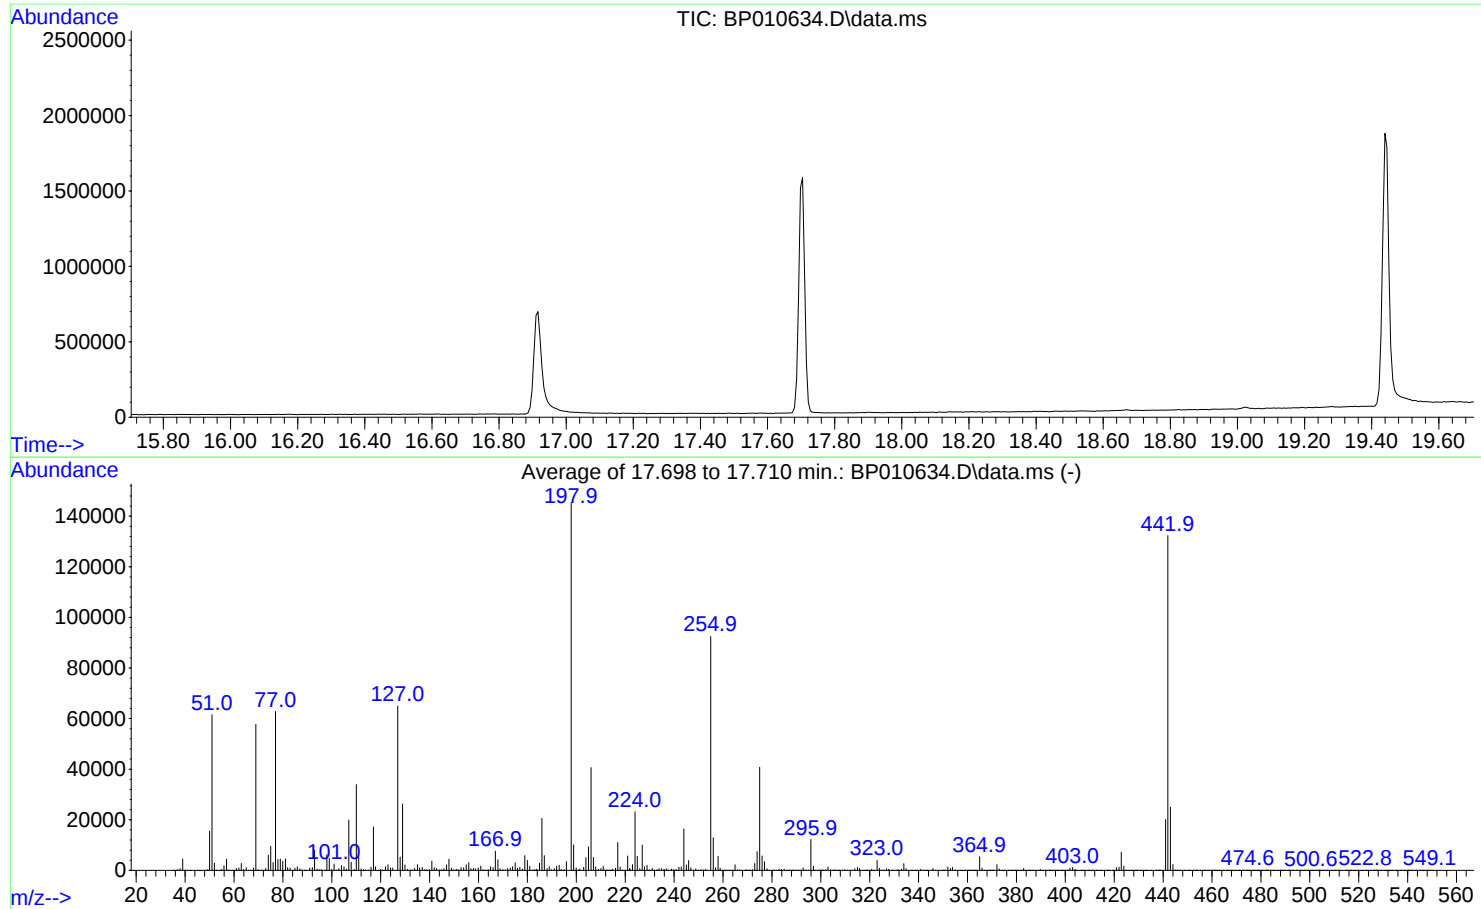




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	61525	PASS
68	69	0.00	2	1.6	944	PASS
69	198	0.00	100	39.7	57700	PASS
70	69	0.00	2	0.3	176	PASS
127	198	10	80	44.7	64924	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145399	PASS
199	198	5	9	6.9	10039	PASS
275	198	10	60	28.0	40717	PASS
365	198	1	100	3.7	5415	PASS
441	198	0.01	100	13.8	20043	PASS
442	442	100	100	100.0	132273	PASS
443	442	15	24	18.9	25015	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
Data File : BP010634.D
Acq On : 31 May 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 01 06:03:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

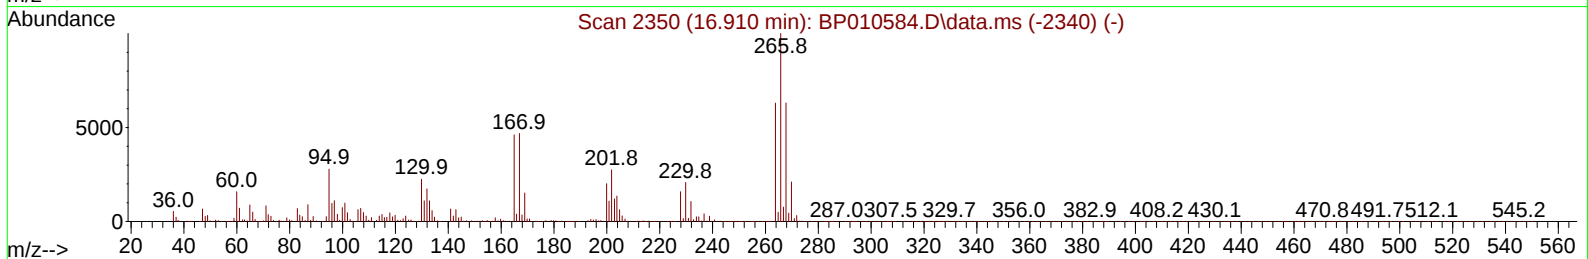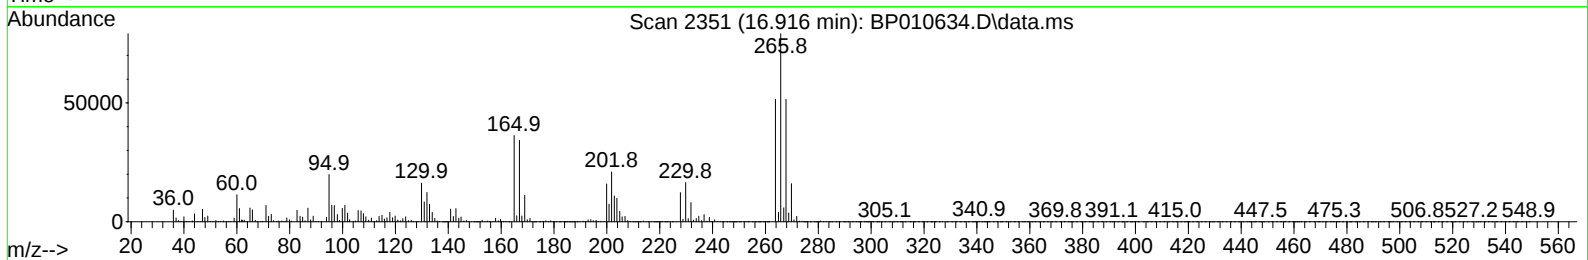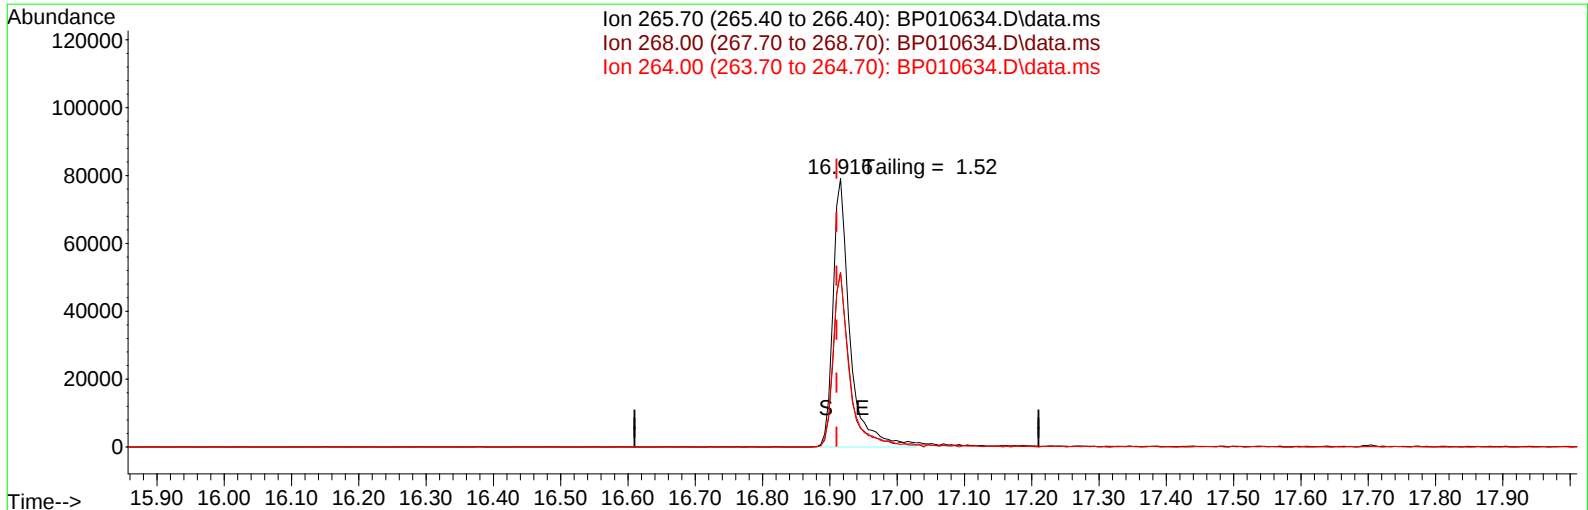

TIC: BP010634.D\data.ms

(70) Pentachlorophenol (C)

16.916min (+ 0.006) 2838105.14 ng




response 137037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.11
264.00	63.00	65.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053122\
Data File : BP010634.D
Acq On : 31 May 2022 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 01 06:03:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 28 02:18:04 2022
Response via : Initial Calibration

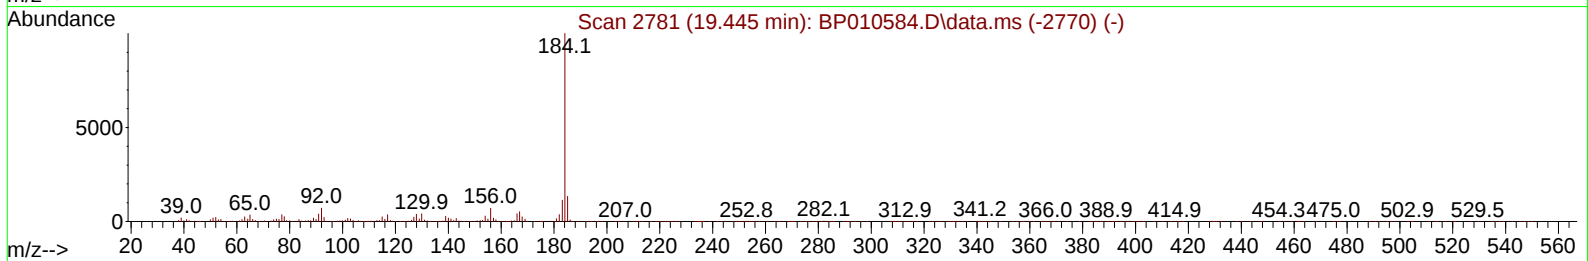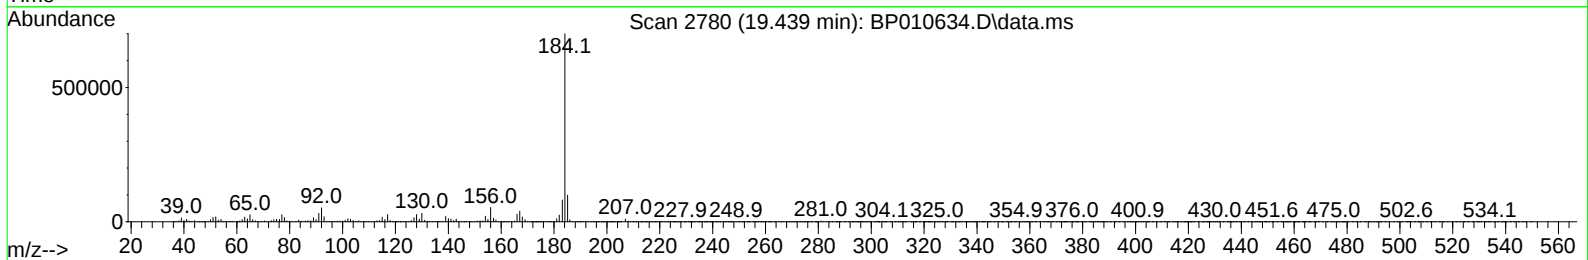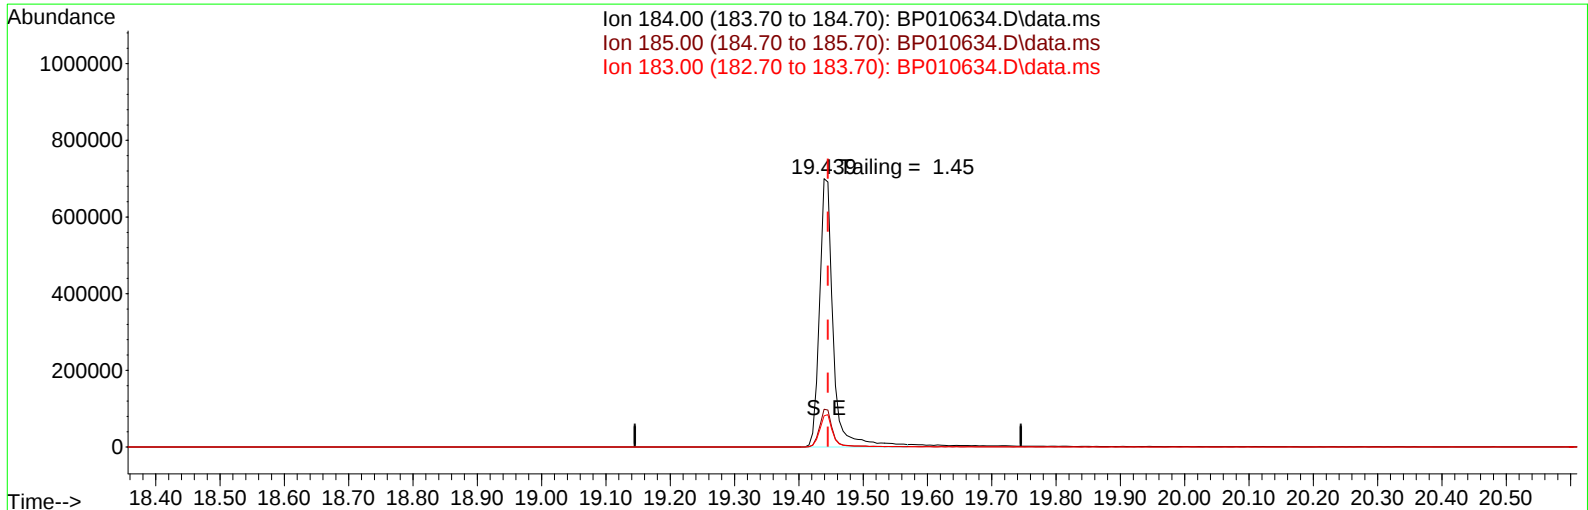

TIC: BP010634.D\data.ms

(77) Benzidine

19.439min (-0.006) 391319.02 ng

response 1052378

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.10
183.00	11.30	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/31/2022	BNA_P	<u>BP010634.D</u>
Compound Name	Response	Retention Time
DDT	522926	20.645
DDD	10232	20.216
DDE	1400	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11632	534558	2.18

Instrument :
BNA_P
ClientSampleId :
DFTPP