

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
 Data File : BP05359.D
 Acq On : 31 May 2023 14:52
 Operator : CG/JU
 Sample : 02851-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0FJ2

Quant Time: May 31 22:42:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 31 14:24:45 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	155696	20.000	ng/ul	0.00
20) Naphthalene-d8	10.934	136	666386	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.751	164	466964	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.504	188	1130062	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1180351	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	1226158	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	27769	6.930	ng/uL	0.00
4) Pyridine-d5	3.858	84	246013	21.658	ng/ul	0.00
7) Phenol-d5	7.258	99	493159	34.114	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	305663	36.610	ng/ul	0.00
11) 2-Chlorophenol-d4	7.628	132	410475	38.619	ng/ul	0.00
15) 4-Methylphenol-d8	8.822	113	430218	37.348	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128	214352	40.935	ng/ul	0.00
24) 2-Nitrophenol-d4	10.010	143	253335	43.480	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.552	165	439826	41.833	ng/ul	0.00
31) 4-Chloroaniline-d4	11.075	131	281406	18.090	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	1555846	44.092	ng/ul	0.00
49) Acenaphthylene-d8	14.445	160	1729289	42.849	ng/ul	0.00
54) 4-Nitrophenol-d4	14.945	143	229528	33.499	ng/ul	0.00
60) Fluorene-d10	15.740	176	1329205	44.642	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.863	200	241135	33.859	ng/ul	0.00
73) Anthracene-d10	17.604	188	2194547	42.410	ng/ul	0.00
81) Pyrene-d10	19.828	212	2751091	40.186	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.974	264	2685783	44.125	ng/ul	0.00
Target Compounds						
18) 4-Methylphenol	8.875	108	112431	8.916	ng/ul	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015359.D
Acq On : 31 May 2023 14:52
Operator : CG/JU
Sample : 02851-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0FJ2

Quant Time: May 31 22:42:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 31 14:24:45 2023
Response via : Initial Calibration

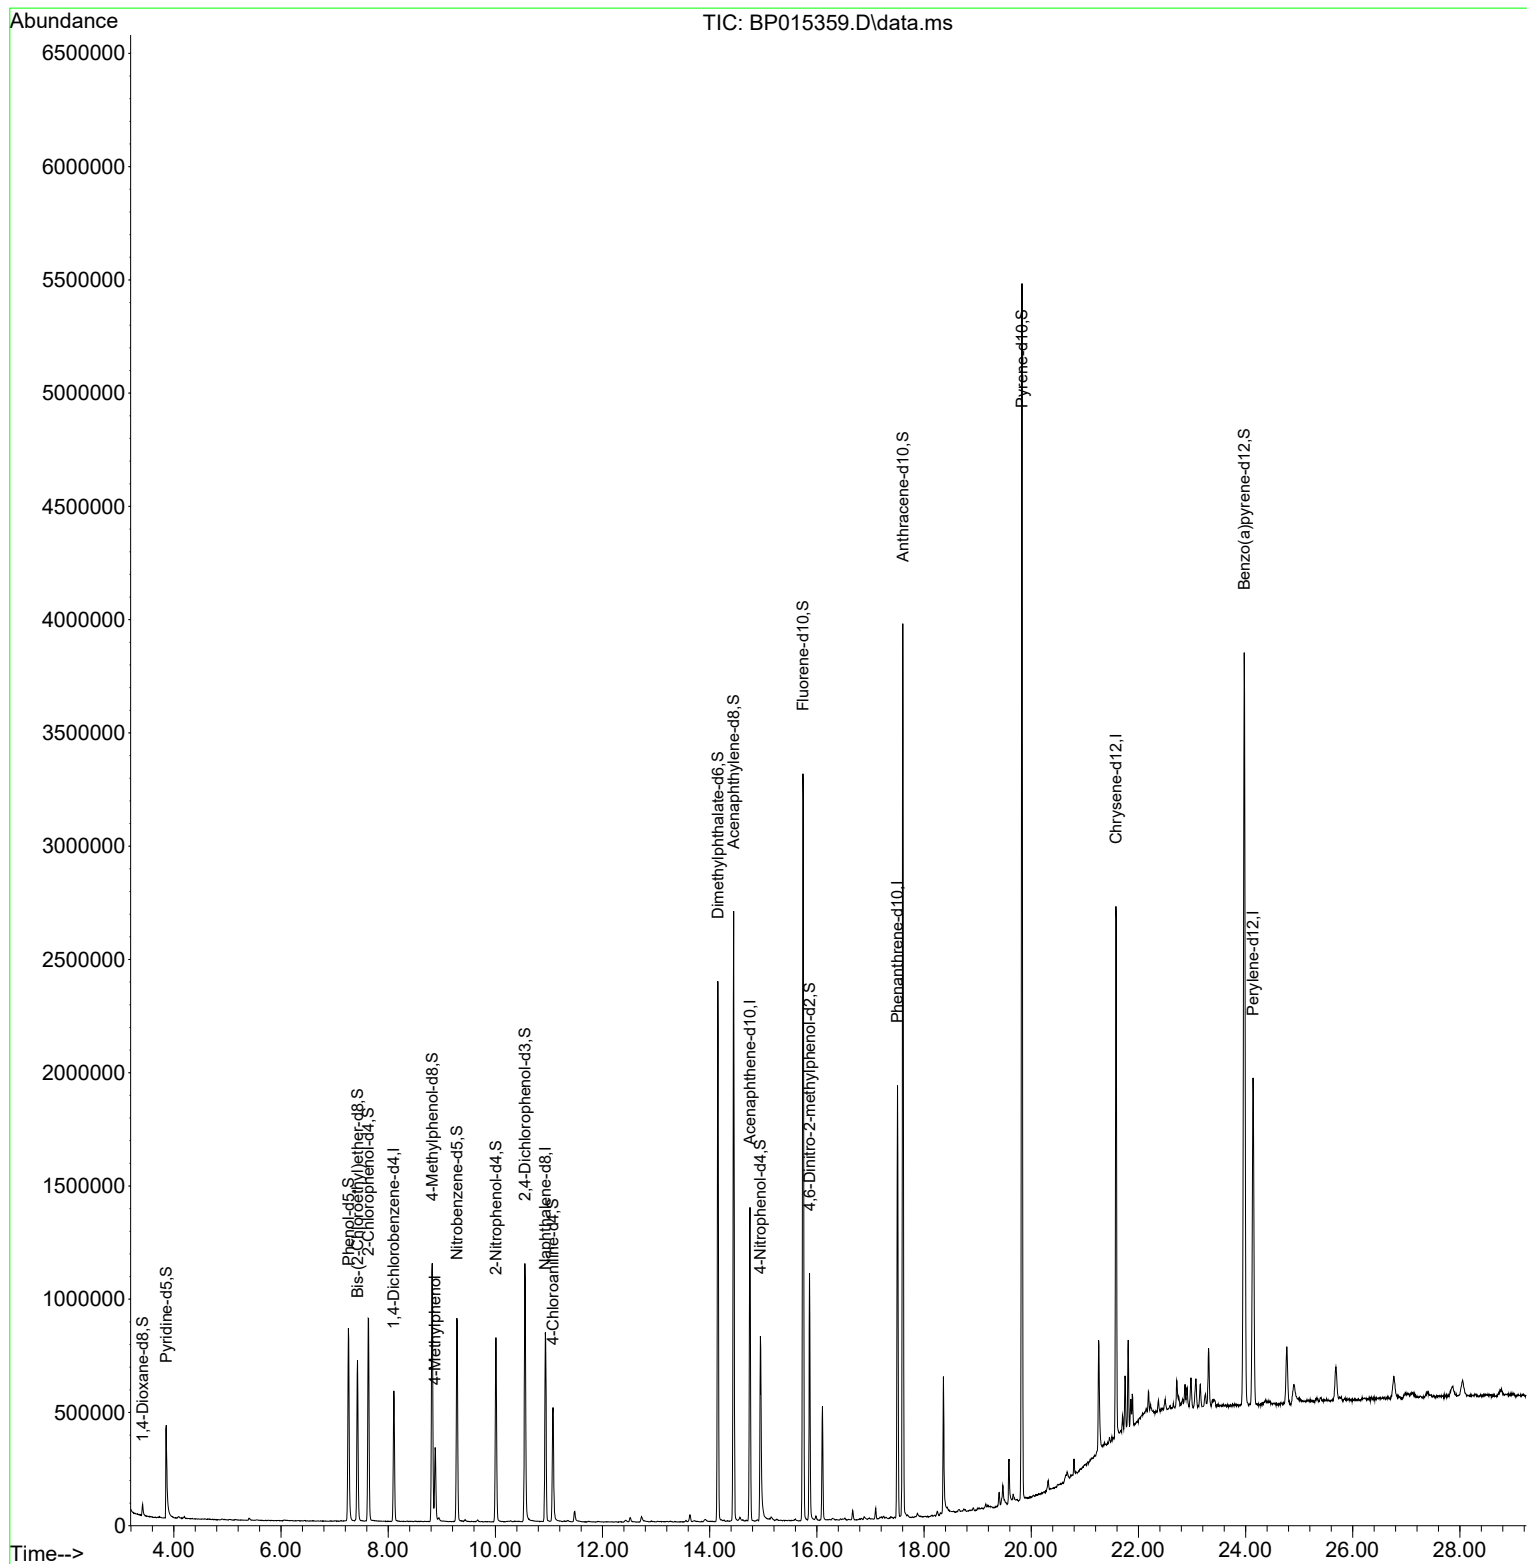

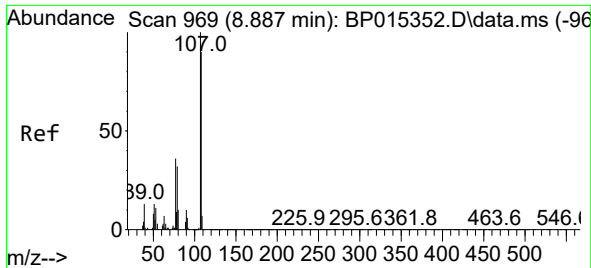

#18
 4-Methylphenol
 Concen: 8.916 ng/ul
 RT: 8.875 min Scan# 90
 Delta R.T. -0.012 min
 Lab File: BP015359.D
 Acq: 31 May 2023 14:52

Instrument :
 BNA_P
 ClientSampleId :
 H0FJ2

Tgt Ion:108 Resp: 112431
 Ion Ratio Lower Upper
 108 100
 107 125.6 88.5 132.7

