

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
 Data File : BP015353.D
 Acq On : 31 May 2023 11:30
 Operator : CG/JU
 Sample : PB153064BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK064

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	35	39	47	rVB	38697	57374	0.96%	0.113%
2	3.852	110	113	135	rBV	485142	859194	14.40%	1.685%
3	4.193	167	171	176	rVB2	6984	12164	0.20%	0.024%
4	7.258	686	692	704	rBV	590028	999724	16.76%	1.961%
5	7.428	715	721	732	rVB	504825	792289	13.28%	1.554%
6	7.634	748	756	769	rBV	634820	1059380	17.76%	2.078%
7	8.105	829	836	847	rBV	499517	814281	13.65%	1.597%
8	8.822	948	958	972	rBV	778914	1364978	22.88%	2.678%
9	9.281	1029	1036	1048	rBV	639184	1085192	18.19%	2.129%
10	10.010	1150	1160	1174	rBV	567045	985284	16.52%	1.933%
11	10.557	1244	1253	1271	rBV	766818	1399579	23.46%	2.746%
12	10.934	1310	1317	1327	rBV	712061	1235106	20.70%	2.423%
13	11.075	1330	1341	1359	rBV	996380	1785199	29.92%	3.502%
14	12.516	1582	1586	1596	rBV4	10052	23991	0.40%	0.047%
15	13.628	1771	1775	1780	rVB4	9246	14697	0.25%	0.029%
16	14.151	1857	1864	1875	rBV	1908316	2581245	43.27%	5.064%
17	14.263	1880	1883	1891	rVB8	4491	9868	0.17%	0.019%
18	14.446	1905	1914	1930	rBV	1999092	2909518	48.77%	5.708%
19	14.751	1957	1966	1974	rBV	1256763	1884050	31.58%	3.696%
20	14.945	1993	1999	2020	rBV	624930	1279844	21.45%	2.511%
21	15.740	2127	2134	2147	rBV	2471378	3680291	61.69%	7.220%
22	15.863	2150	2155	2170	rVV	1005071	1431717	24.00%	2.809%
23	15.981	2170	2175	2181	rVB5	13390	26369	0.44%	0.052%
24	17.504	2427	2434	2444	rBV	1775448	2554646	42.82%	5.011%
25	17.604	2445	2451	2463	rVV2	3030379	4327185	72.53%	8.489%
26	18.369	2578	2581	2588	rBV9	4571	11970	0.20%	0.023%
27	19.404	2753	2757	2762	rBV3	47884	65790	1.10%	0.129%
28	19.475	2765	2769	2773	rVV	34685	51937	0.87%	0.102%
29	19.828	2823	2829	2839	rBV	4102571	5488525	92.00%	10.767%
30	21.586	3123	3128	3135	rBV	2398461	3103757	52.03%	6.089%
31	23.980	3527	3535	3548	rVB2	2829460	5965662	100.00%	11.703%
32	24.145	3556	3563	3572	rVB	1483217	3115050	52.22%	6.111%




Sum of corrected areas: 50975856

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015353.D
Acq On : 31 May 2023 11:30
Operator : CG/JU
Sample : PB153064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

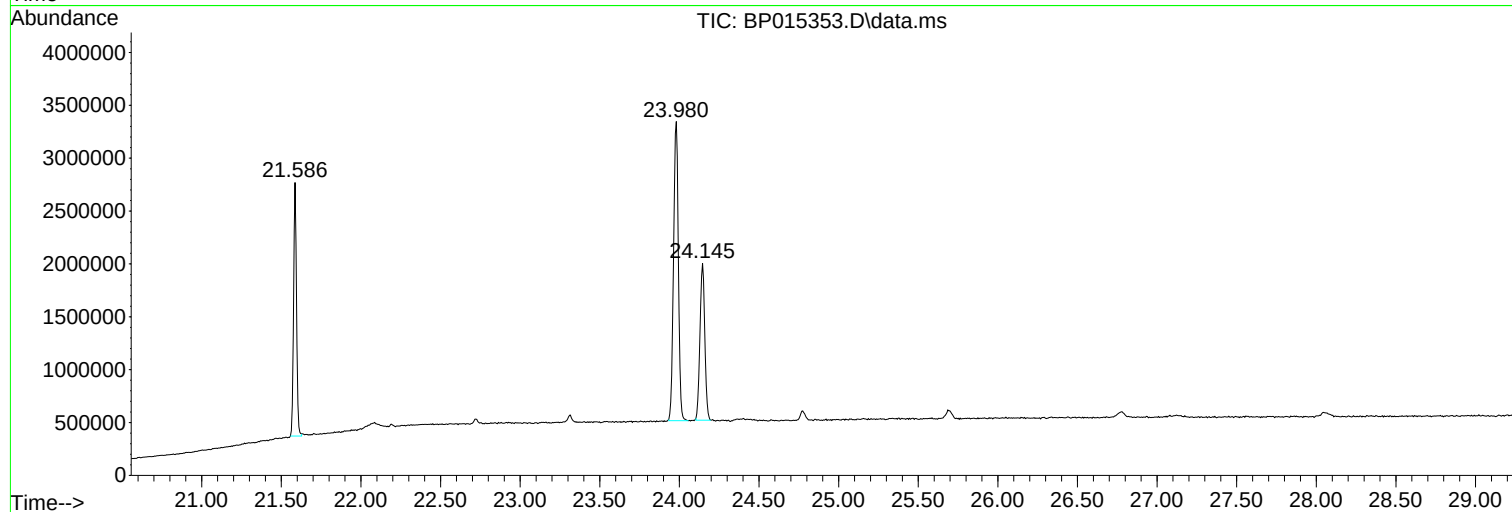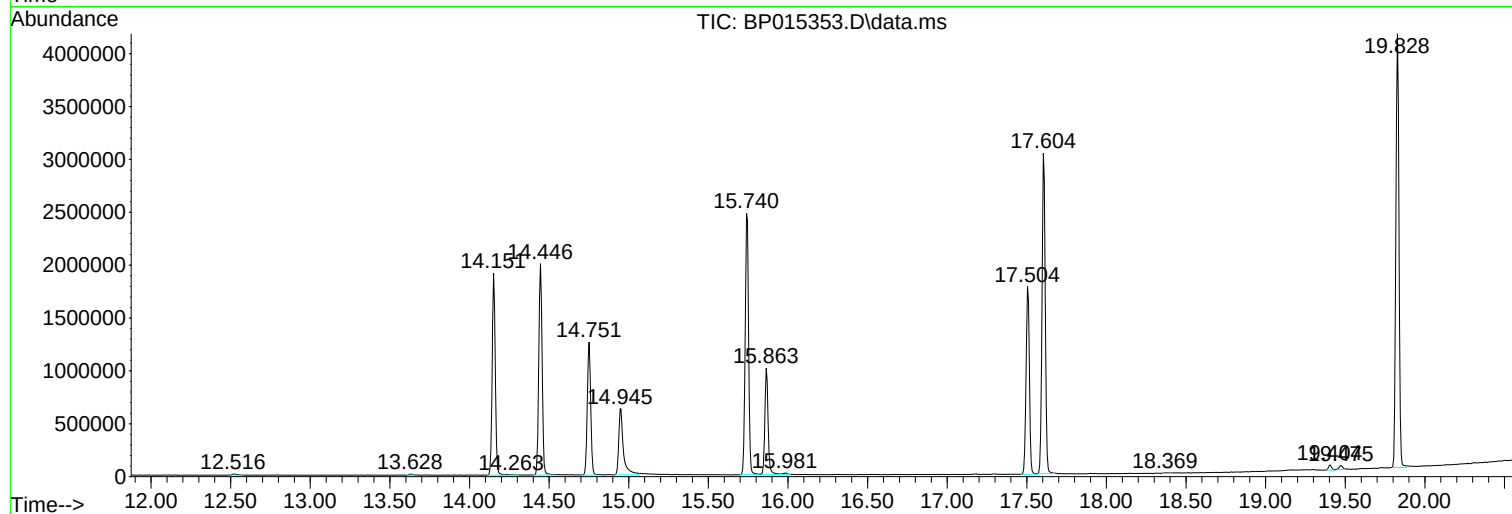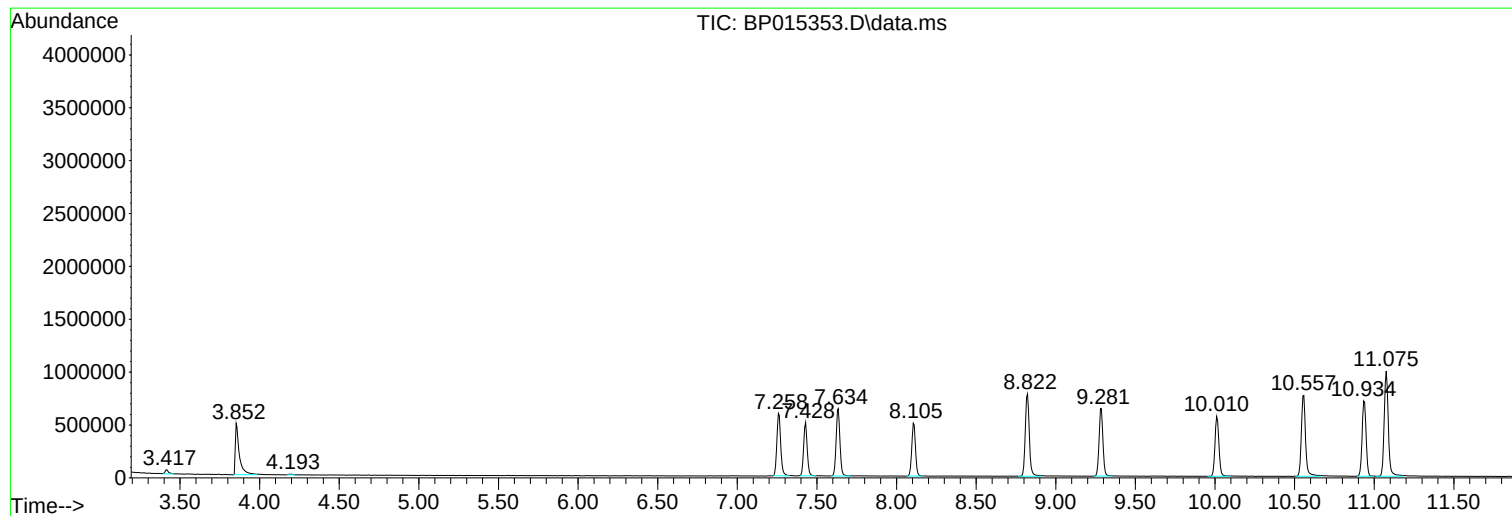

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015353.D
Acq On : 31 May 2023 11:30
Operator : CG/JU
Sample : PB153064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015353.D
Acq On : 31 May 2023 11:30
Operator : CG/JU
Sample : PB153064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK064

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------