

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
 Data File : BP015371.D
 Acq On : 31 May 2023 22:12
 Operator : CG/JU
 Sample : PB153106BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	5	7	12	rVB2	12679	18997	0.34%	0.035%
2	3.416	34	39	49	rVB	53867	84601	1.51%	0.155%
3	3.858	112	114	133	rBV	257654	450003	8.06%	0.822%
4	4.193	166	171	175	rBV4	9923	13341	0.24%	0.024%
5	7.257	685	692	703	rBV	800936	1321146	23.65%	2.413%
6	7.422	714	720	733	rBV	669131	1072893	19.21%	1.959%
7	7.628	748	755	767	rBV	864065	1396234	25.00%	2.550%
8	8.104	827	836	850	rBV	628216	1014026	18.15%	1.852%
9	8.816	950	957	975	rBV	1063831	1798034	32.19%	3.284%
10	9.281	1028	1036	1050	rBV	890638	1479220	26.48%	2.701%
11	10.010	1151	1160	1175	rBV	778339	1334630	23.89%	2.437%
12	10.551	1244	1252	1268	rBV	1001363	1834079	32.84%	3.350%
13	10.934	1309	1317	1325	rBV	938219	1564221	28.01%	2.857%
14	11.069	1333	1340	1353	rBV	275349	549258	9.83%	1.003%
15	12.516	1579	1586	1595	rBV2	15858	37151	0.67%	0.068%
16	13.545	1756	1761	1764	rBV7	2898	5710	0.10%	0.010%
17	13.628	1769	1775	1783	rBV	33230	54680	0.98%	0.100%
18	13.728	1787	1792	1796	rBV6	3962	7381	0.13%	0.013%
19	14.151	1854	1864	1877	rBV	2137826	3002363	53.75%	5.483%
20	14.439	1906	1913	1927	rBV2	2345548	3526831	63.14%	6.441%
21	14.745	1958	1965	1976	rBV	1496119	2197524	39.34%	4.013%
22	14.857	1980	1984	1991	rBV9	4099	8723	0.16%	0.016%
23	14.945	1991	1999	2019	rBV	839248	1577790	28.25%	2.881%
24	15.145	2032	2033	2041	rVB7	5501	6955	0.12%	0.013%
25	15.739	2126	2134	2145	rBV	2989954	4265962	76.38%	7.791%
26	15.857	2148	2154	2168	rVV	1113544	1673307	29.96%	3.056%
27	15.975	2171	2174	2184	rVB4	17206	30020	0.54%	0.055%
28	16.528	2262	2268	2273	rVB9	4116	7629	0.14%	0.014%
29	17.175	2374	2378	2383	rVB8	5485	8461	0.15%	0.015%
30	17.286	2392	2397	2404	rBV4	5815	11188	0.20%	0.020%
31	17.498	2427	2433	2441	rBV	1898202	2754024	49.31%	5.030%
32	17.598	2444	2450	2470	rVB2	3192189	4693689	84.03%	8.572%
33	18.145	2540	2543	2548	rVB7	9601	11922	0.21%	0.022%
34	18.357	2577	2579	2586	rBV7	5782	8736	0.16%	0.016%
35	19.398	2751	2756	2761	rBV	47745	69114	1.24%	0.126%
36	19.469	2763	2768	2771	rBV	44636	61944	1.11%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015371.D
Acq On : 31 May 2023 22:12
Operator : CG/JU
Sample : PB153106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK106

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	19.822	2822	2828	2838	rBV	4265529	5585483	100.00%	10.201%
38	21.580	3121	3127	3133	rBV	2254489	3008974	53.87%	5.495%
39	23.968	3525	3533	3542	rVB2	2665642	5346393	95.72%	9.764%
40	24.127	3553	3560	3572	rVB	1313320	2863754	51.27%	5.230%




Sum of corrected areas: 54756391

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP05123\
Data File : BP015371.D
Acq On : 31 May 2023 22:12
Operator : CG/JU
Sample : PB153106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK106

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

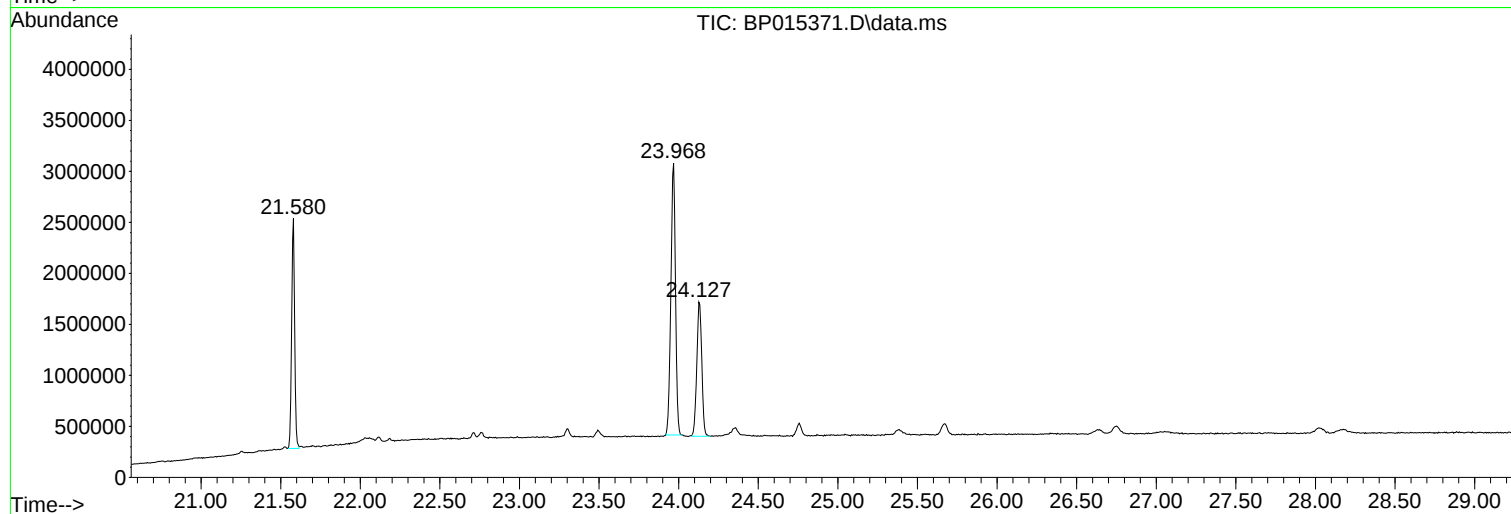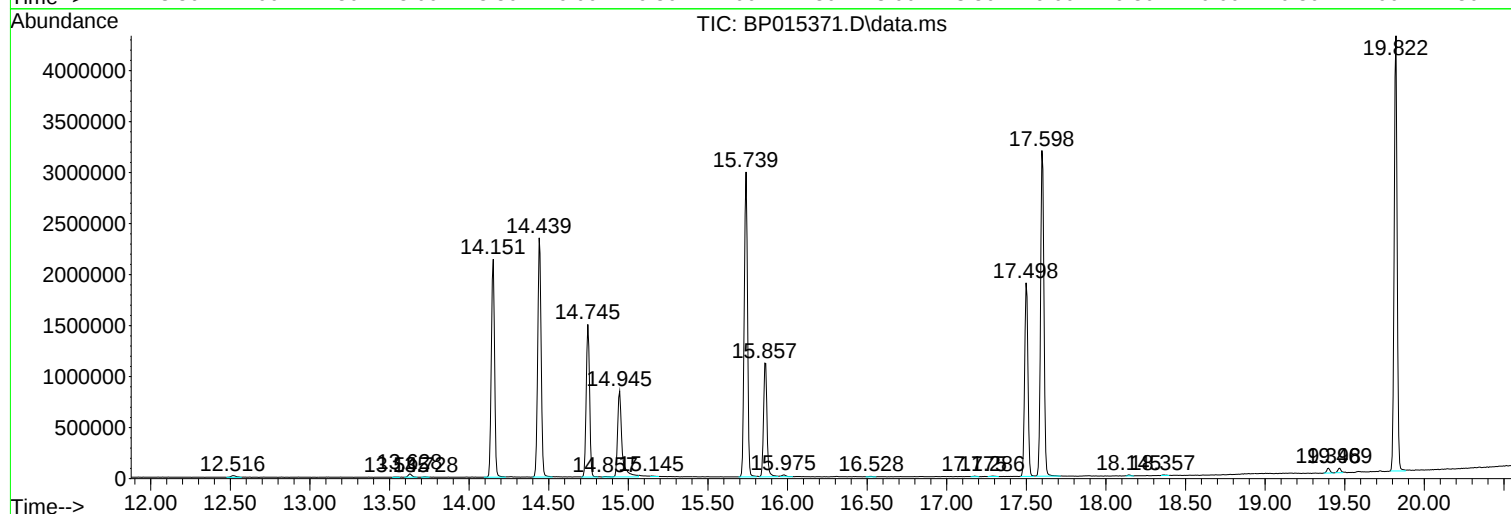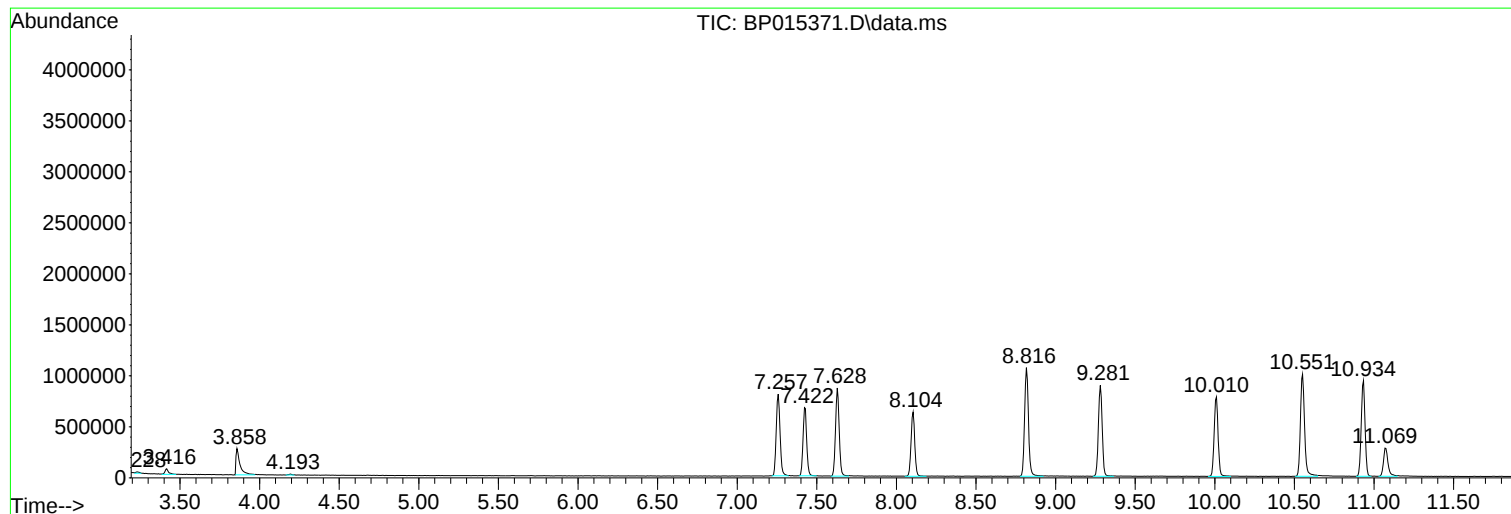

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015371.D
Acq On : 31 May 2023 22:12
Operator : CG/JU
Sample : PB153106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK106

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015371.D
Acq On : 31 May 2023 22:12
Operator : CG/JU
Sample : PB153106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK106

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------