

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
 Data File : BP015372.D
 Acq On : 31 May 2023 22:45
 Operator : CG/JU
 Sample : PB153144BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	35	39	46	rVB	54399	73854	1.21%	0.121%
2	3.852	110	113	136	rBV	691296	1121249	18.40%	1.844%
3	4.193	168	171	176	rVB2	12248	14582	0.24%	0.024%
4	7.258	685	692	706	rBV	866412	1431166	23.49%	2.353%
5	7.422	714	720	731	rBV	708010	1133039	18.59%	1.863%
6	7.628	748	755	767	rBV	922165	1486472	24.39%	2.444%
7	8.105	827	836	847	rBV	660111	1058356	17.37%	1.740%
8	8.816	949	957	975	rBV	1158882	1926063	31.61%	3.167%
9	9.281	1028	1036	1050	rBV	951880	1573376	25.82%	2.587%
10	10.010	1152	1160	1174	rBV	822913	1425799	23.40%	2.344%
11	10.551	1243	1252	1268	rBV	1085588	1951844	32.03%	3.209%
12	10.934	1308	1317	1329	rVB	973567	1651700	27.11%	2.716%
13	11.069	1332	1340	1364	rBV	1162817	2105643	34.55%	3.462%
14	12.516	1578	1586	1595	rBV	17976	38832	0.64%	0.064%
15	13.628	1771	1775	1783	rVB2	21445	34224	0.56%	0.056%
16	14.151	1857	1864	1878	rBV	2333090	3266184	53.60%	5.370%
17	14.440	1906	1913	1929	rBV	2510578	3760293	61.71%	6.183%
18	14.745	1958	1965	1977	rBV	1653641	2331233	38.26%	3.833%
19	14.857	1980	1984	1991	rVB10	4422	8195	0.13%	0.013%
20	14.939	1991	1998	2024	rBV	940306	1770126	29.05%	2.910%
21	15.151	2031	2034	2040	rVB8	6609	10344	0.17%	0.017%
22	15.739	2127	2134	2148	rBV	3111979	4550188	74.67%	7.481%
23	15.857	2148	2154	2168	rVV	1285502	1848896	30.34%	3.040%
24	15.975	2170	2174	2180	rVB2	16016	29881	0.49%	0.049%
25	16.516	2263	2266	2273	rBV9	5209	8781	0.14%	0.014%
26	17.169	2373	2377	2383	rVB9	6341	10460	0.17%	0.017%
27	17.286	2395	2397	2401	rVB3	4868	6194	0.10%	0.010%
28	17.498	2426	2433	2441	rBV	2027263	2924001	47.98%	4.808%
29	17.598	2443	2450	2464	rVV	3665269	5168658	84.82%	8.498%
30	18.363	2576	2580	2584	rBV6	7096	10993	0.18%	0.018%
31	19.392	2752	2755	2761	rVB	48752	65615	1.08%	0.108%
32	19.463	2763	2767	2772	rBV	47072	66863	1.10%	0.110%
33	19.822	2822	2828	2840	rBV	4551855	6093684	100.00%	10.019%
34	21.574	3121	3126	3134	rBV	2366944	3201752	52.54%	5.264%
35	23.963	3524	3532	3542	rVB2	2740024	5727777	94.00%	9.418%
36	24.127	3553	3560	3569	rVB	1382097	2933828	48.15%	4.824%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015372.D
Acq On : 31 May 2023 22:45
Operator : CG/JU
Sample : PB153144BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK144

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 60820145

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015372.D
Acq On : 31 May 2023 22:45
Operator : CG/JU
Sample : PB153144BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

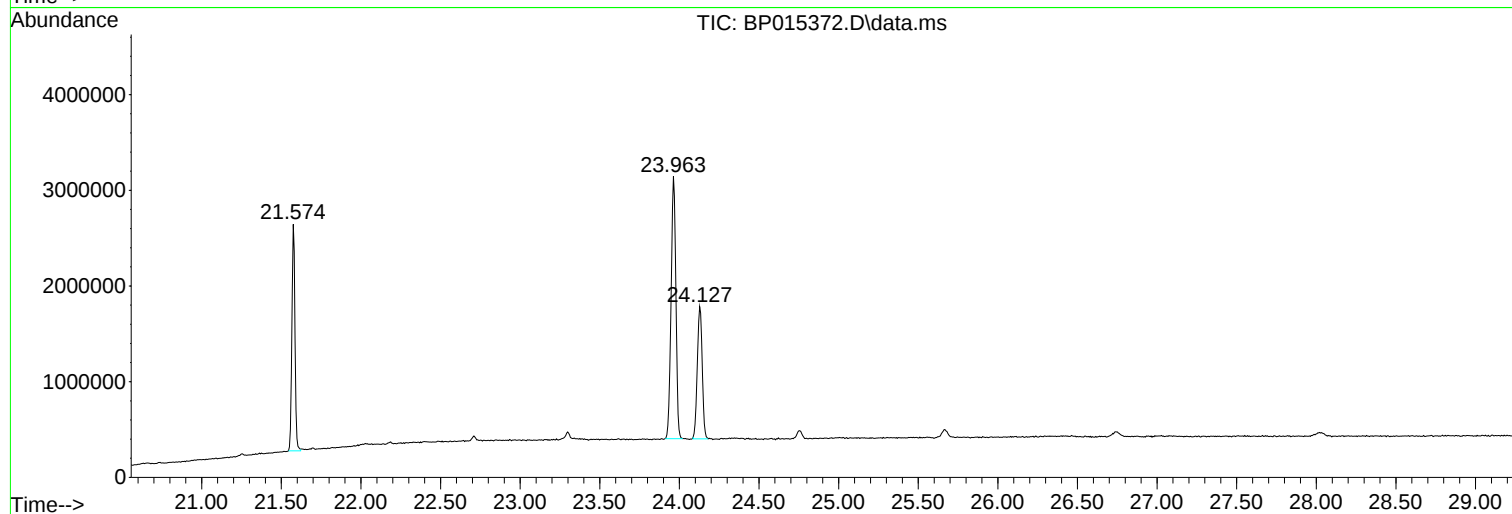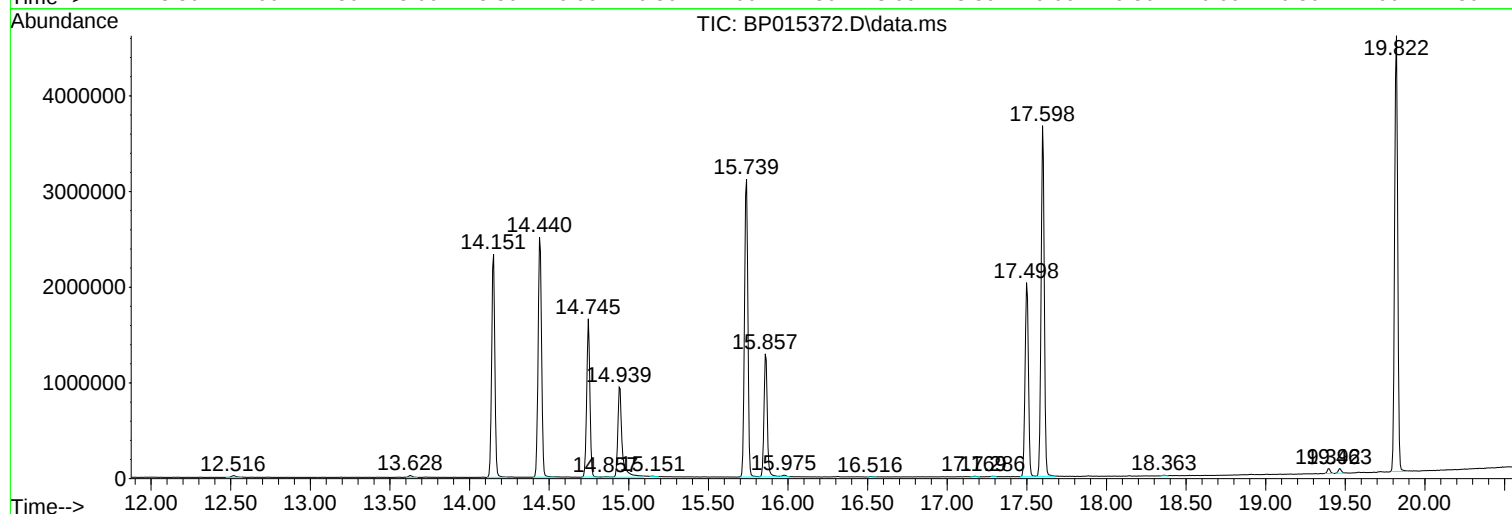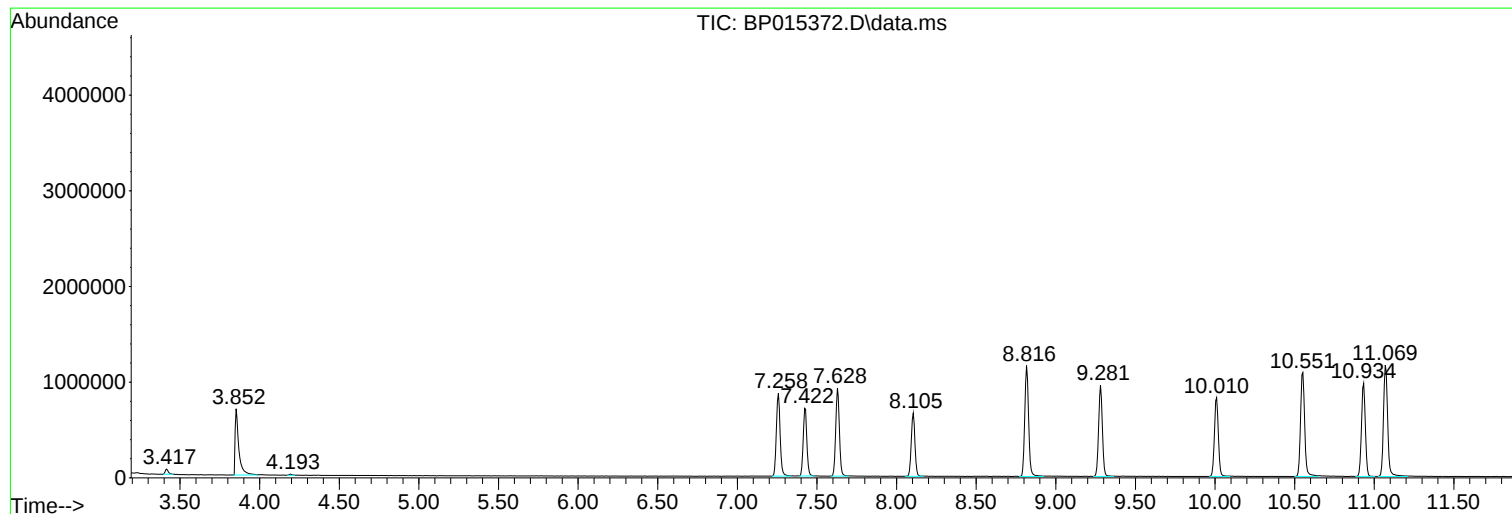

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015372.D
Acq On : 31 May 2023 22:45
Operator : CG/JU
Sample : PB153144BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP053123\
Data File : BP015372.D
Acq On : 31 May 2023 22:45
Operator : CG/JU
Sample : PB153144BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------