
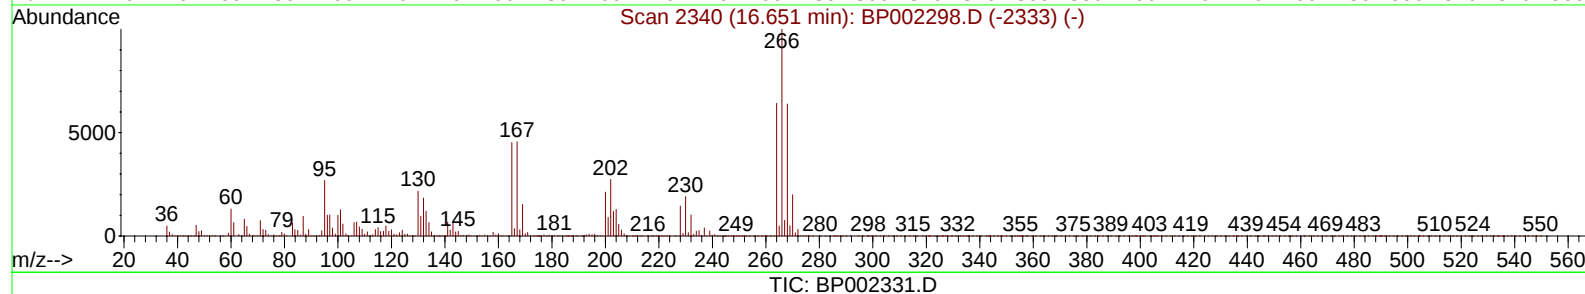
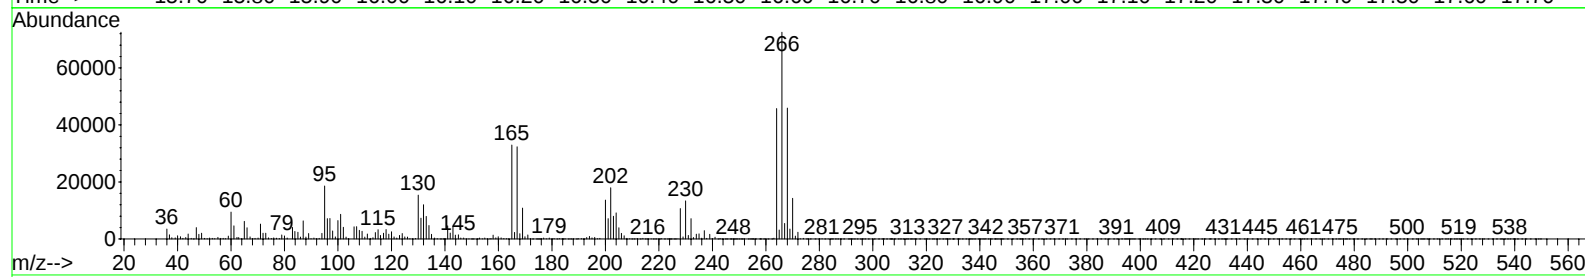


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060120\
Data File : BP002331.D
Acq On : 01 Jun 2020 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 16:35:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 15:09:03 2020
Response via : Initial Calibration

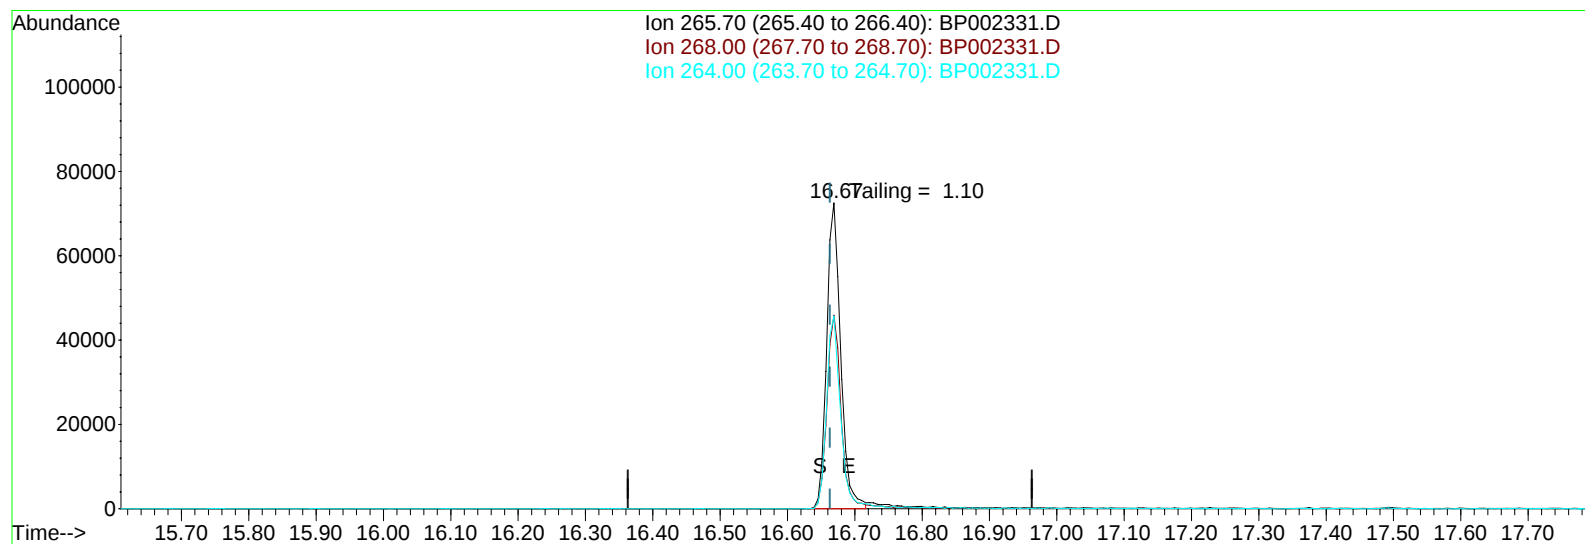

(70) Pentachlorophenol (C)




16.669min (+0.006) 267165.53ng

response 108300

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.34
264.00	60.40	63.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060120\
 Data File : BP002331.D
 Acq On : 01 Jun 2020 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 16:35:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 29 15:09:03 2020
 Response via : Initial Calibration

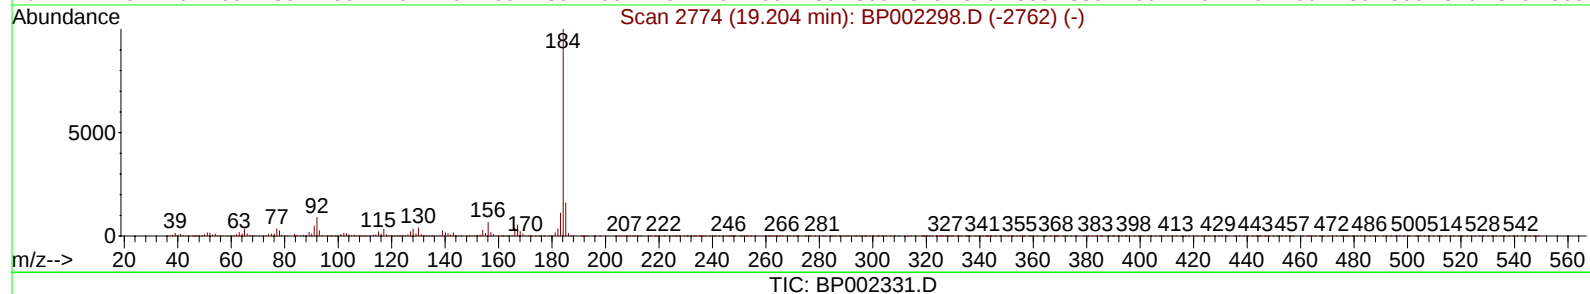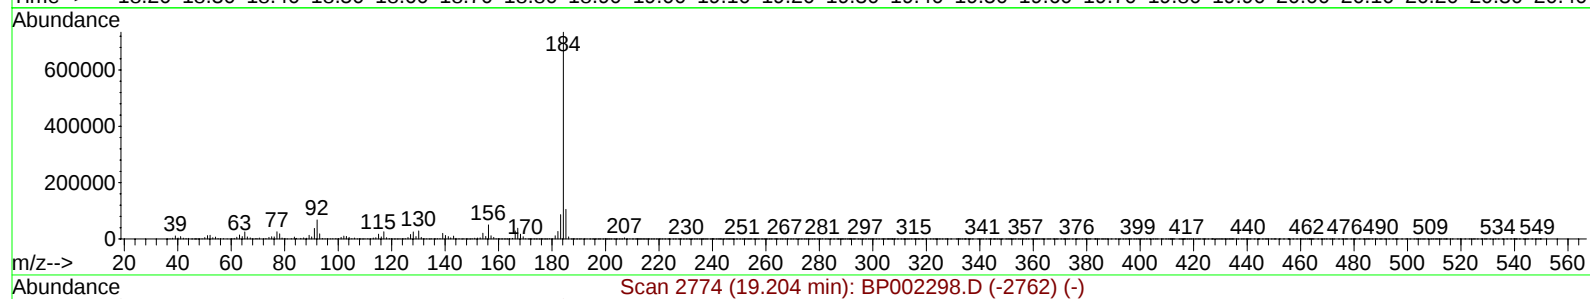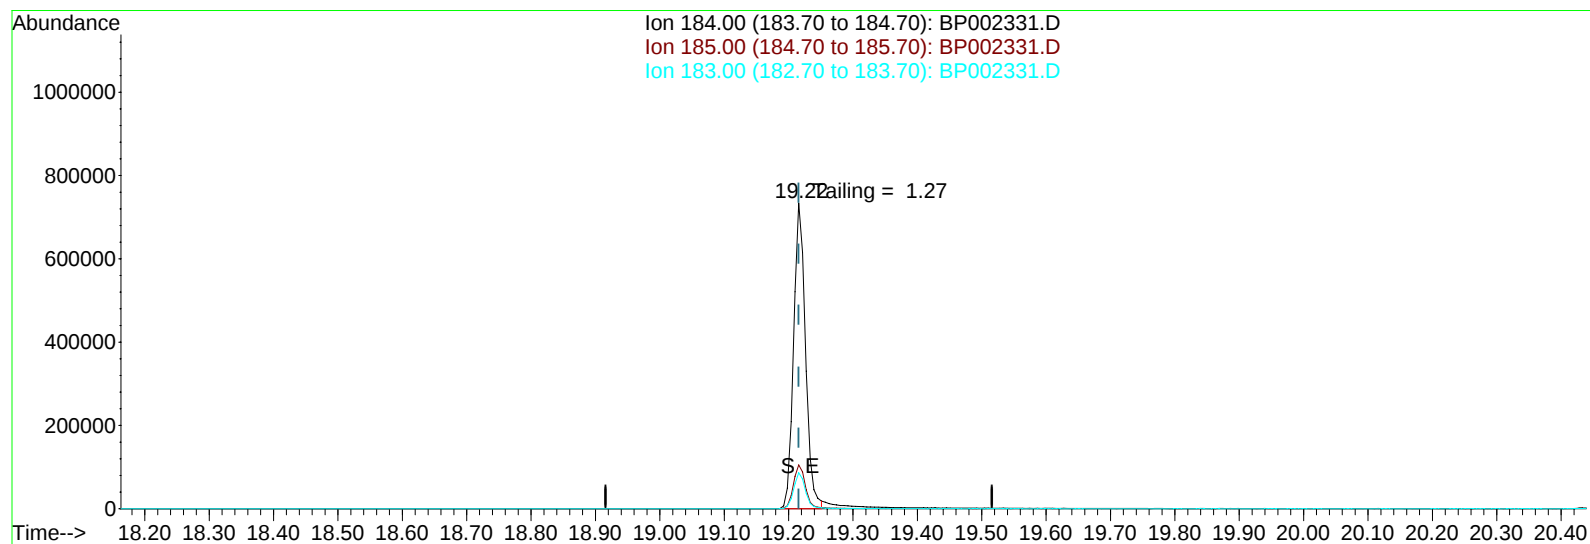

(77) Benzidine

19.216min (+0.000) 174701.74ng m

response 975637

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.35
183.00	11.40	11.78
0.00	0.00	0.00