

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP060120\
 Data File : BP002333.D
 Acq On : 01 Jun 2020 11:47
 Operator : CG/JU
 Sample : PB129172BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB129172BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	391	397	412	rBV	3835149	5702248	46.18%	8.896%
2	6.793	656	664	683	rBV	3717865	5932561	48.04%	9.255%
3	7.605	795	802	815	rBV	926505	1437797	11.64%	2.243%
4	7.928	849	857	866	rBV	3164009	5210548	42.20%	8.128%
5	8.752	989	997	1016	rBV	2460976	4094079	33.16%	6.387%
6	10.381	1265	1274	1285	rBV	1176172	1955884	15.84%	3.051%
7	12.869	1690	1697	1714	rBV	5500359	8506984	68.89%	13.271%
8	14.251	1924	1932	1943	rBV	1736682	2550618	20.66%	3.979%
9	15.751	2180	2187	2207	rBV	4073449	6036361	48.89%	9.417%
10	17.010	2391	2401	2413	rBV	2152757	3103434	25.13%	4.841%
11	19.598	2835	2841	2859	rBV	9239717	12348011	100.00%	19.263%
12	21.110	3093	3098	3108	rBV2	2770705	3557340	28.81%	5.549%
13	23.321	3468	3474	3486	rVB	2007971	3666606	29.69%	5.720%




Sum of corrected areas: 64102471

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP060120\
Data File : BP002333.D
Acq On : 01 Jun 2020 11:47
Operator : CG/JU
Sample : PB129172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129172BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

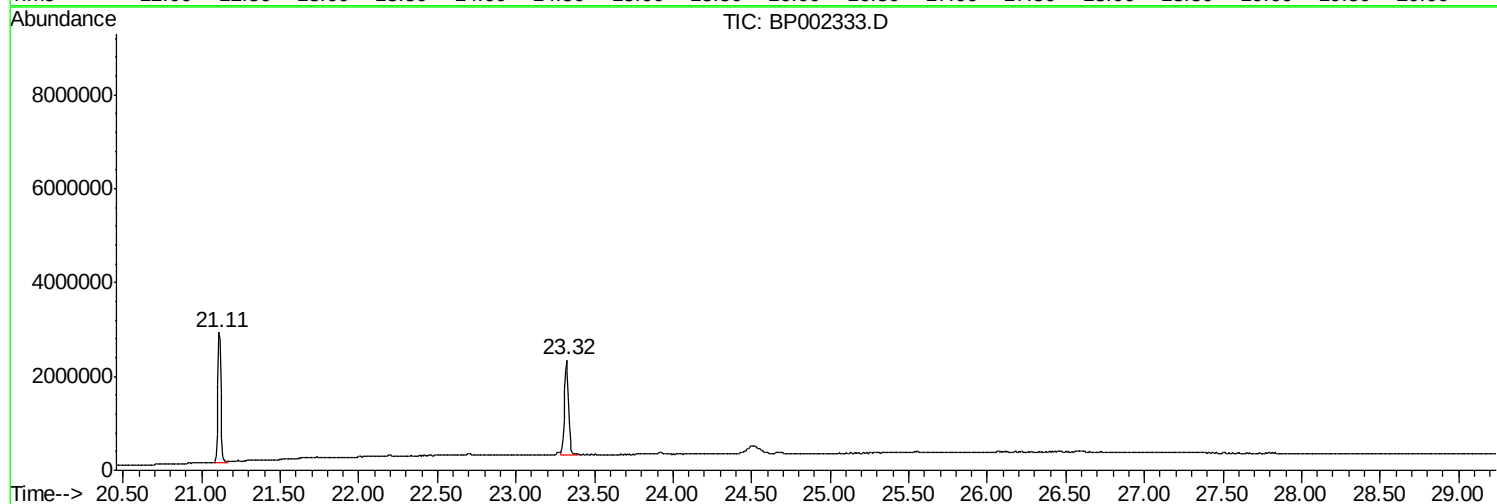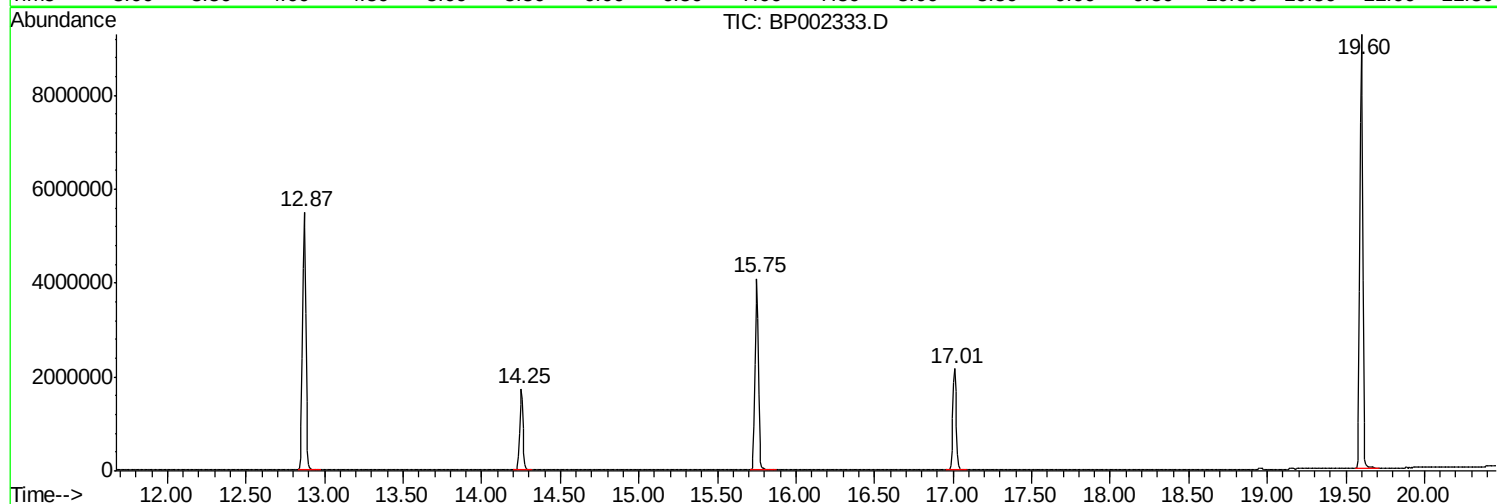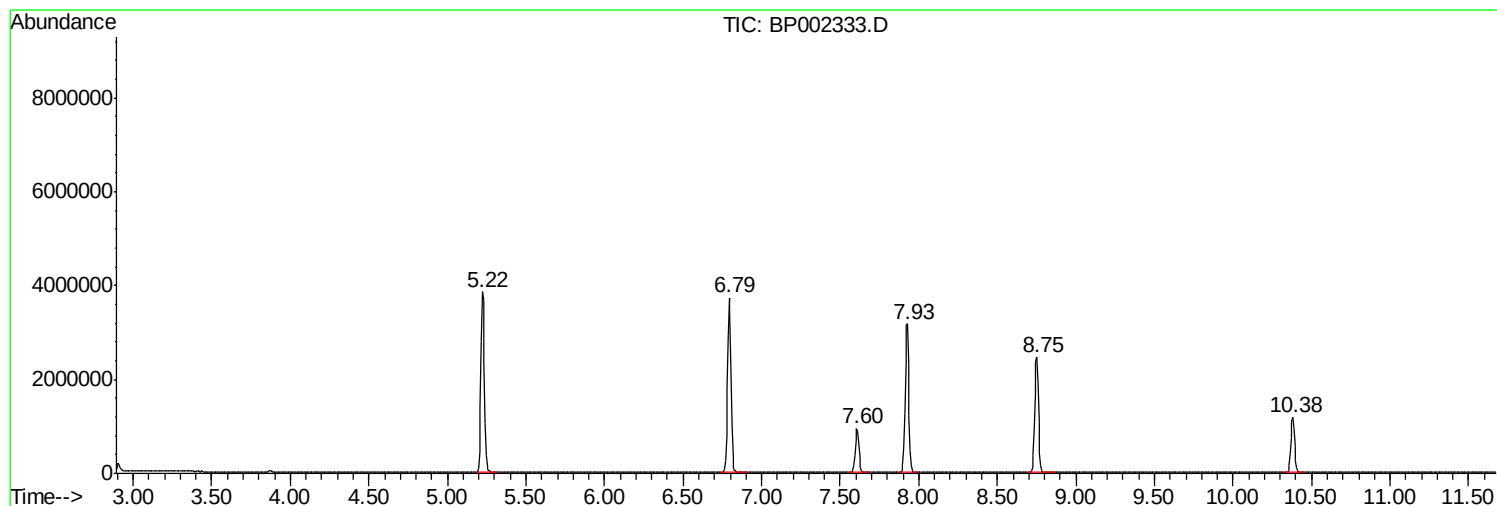

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP060120\
Data File : BP002333.D
Acq On : 01 Jun 2020 11:47
Operator : CG/JU
Sample : PB129172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129172BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP060120\
Data File : BP002333.D
Acq On : 01 Jun 2020 11:47
Operator : CG/JU
Sample : PB129172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB129172BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc