


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP060120\
 Data File : BP002331.D
 Acq On : 01 Jun 2020 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP052720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 29 15:09:03 2020

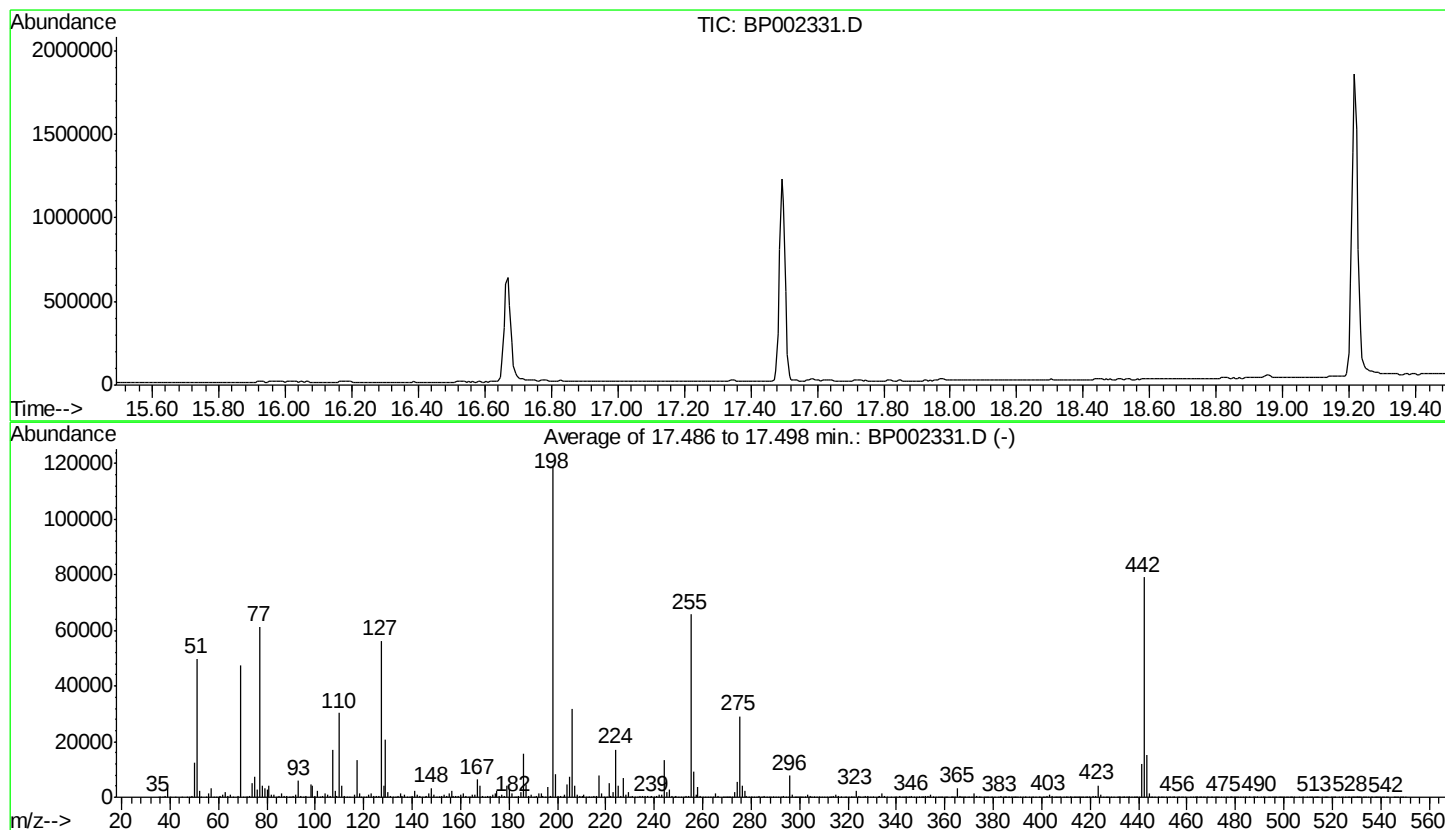

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	49920	PASS
68	69	0.00	2	1.4	667	PASS
69	198	0.00	100	40.0	47660	PASS
70	69	0.00	2	0.4	181	PASS
127	198	10	80	47.2	56344	PASS
197	198	0.00	2	0.3	369	PASS
198	198	100	100	100.0	119272	PASS
199	198	5	9	6.9	8206	PASS
275	198	10	60	24.3	29013	PASS
365	198	1	100	2.9	3432	PASS
441	198	0.01	100	10.1	12043	PASS
442	198	50	100	66.3	79045	PASS
443	442	15	24	19.3	15222	PASS