
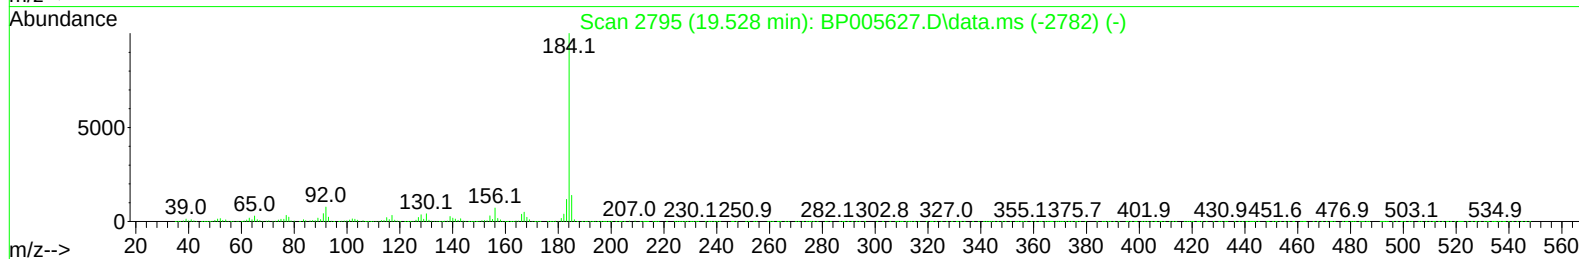
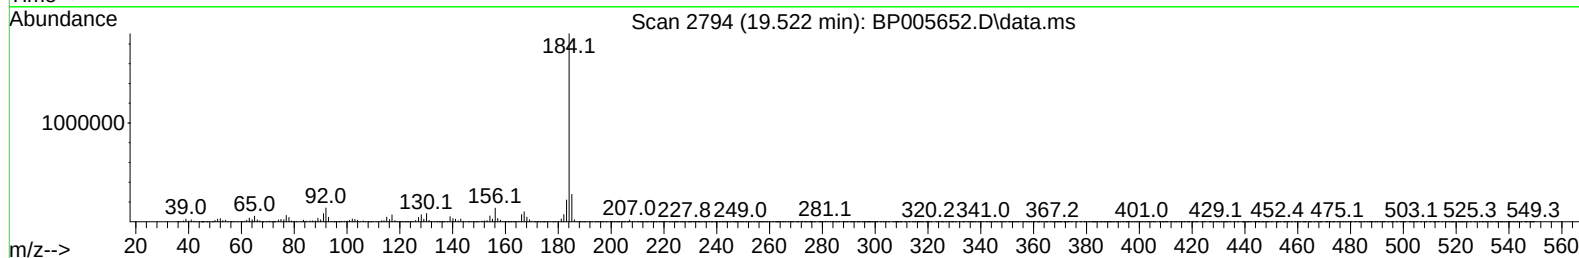


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\
Data File : BP005652.D
Acq On : 01 Jun 2021 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 11:16:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration



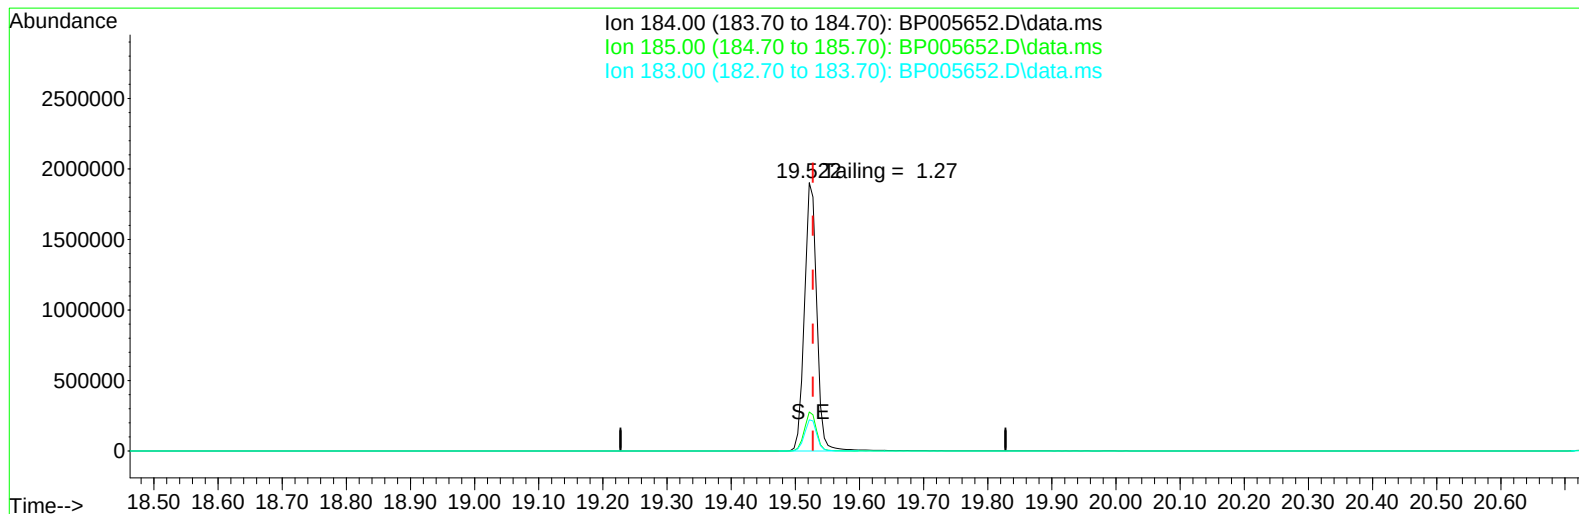


TIC: BP005652.D\data.ms

(77) Benzidine**19.522min (-0.006) 188155.35 ng****response 2551347**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.59
183.00	12.30	11.62
0.00	0.00	0.00

Quant Time: Jun 01 11:16:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

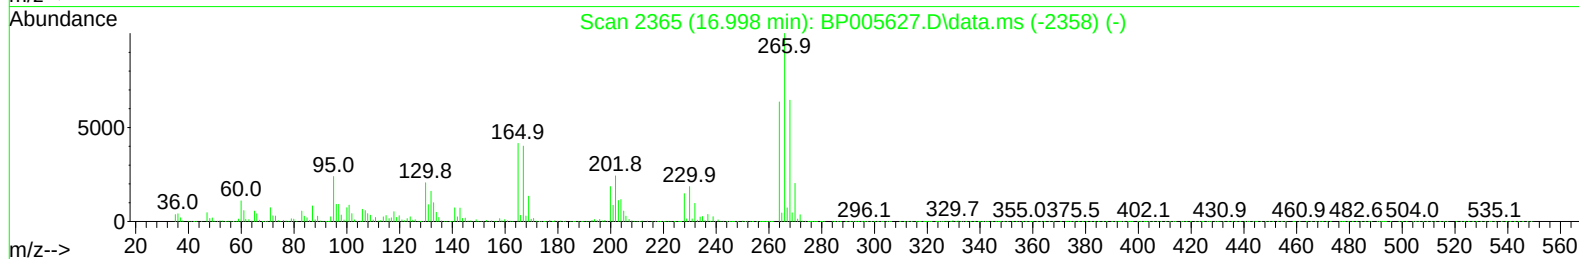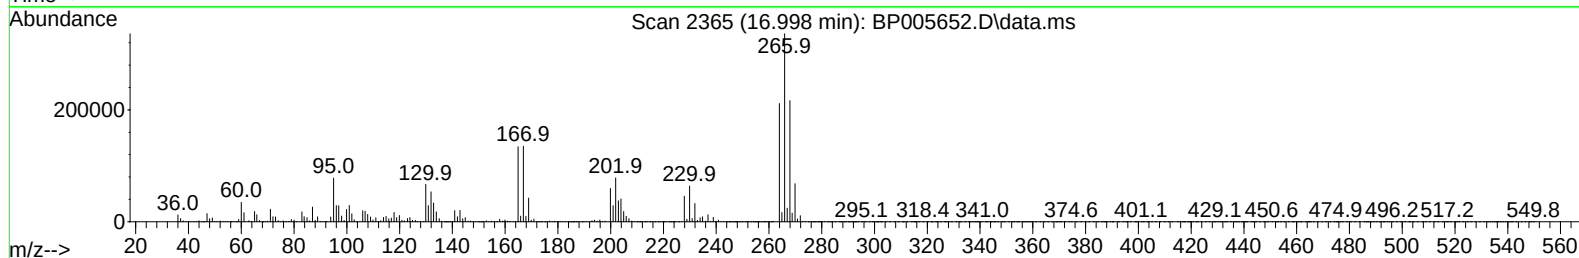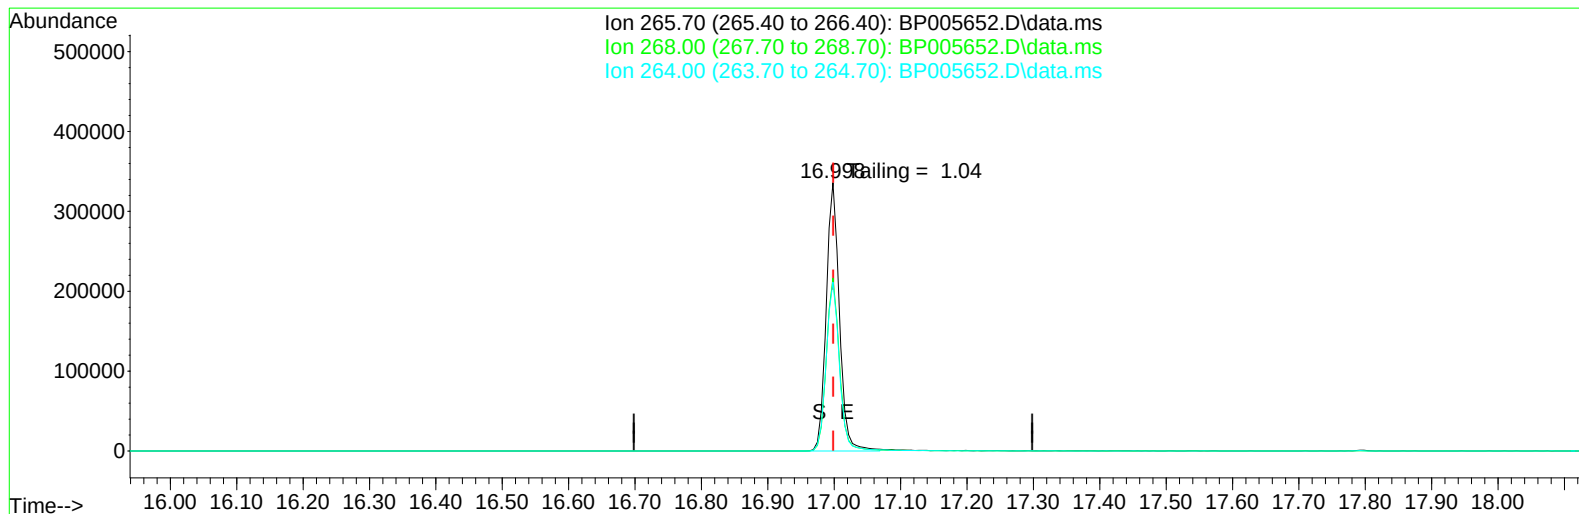

TIC: BP005652.D\data.ms

16.998min (-0.000) 182785.02 ng

response **466813**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------

268.00	61.70	64.42
--------	-------	-------

264.00	67.10	62.90
--------	-------	-------

0.00 0.00 0.00