

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\
 Data File : BP005658.D
 Acq On : 01 Jun 2021 15:17
 Operator : CG/JU
 Sample : PB136714TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB136714TB

Quant Time: Jun 01 15:54:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	193597	20.00	ng	0.00
21) Naphthalene-d8	10.793	136	759694	20.00	ng	# 0.00
39) Acenaphthene-d10	14.604	164	449918	20.00	ng	0.00
64) Phenanthrene-d10	17.345	188	959640	20.00	ng	# 0.00
76) Chrysene-d12	21.416	240	982529	20.00	ng	# 0.00
86) Perylene-d12	23.857	264	1027049	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.546	112	1489820	119.64	ng	0.00
7) Phenol-d6	7.146	99	1775591	104.60	ng	0.00
23) Nitrobenzene-d5	9.146	82	1092158	79.95	ng	0.00
42) 2,4,6-Tribromophenol	16.092	330	682422	118.29	ng	0.00
45) 2-Fluorobiphenyl	13.240	172	2441536	71.82	ng	0.00
79) Terphenyl-d14	19.892	244	4086078	78.04	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\
Data File : BP005658.D
Acq On : 01 Jun 2021 15:17
Operator : CG/JU
Sample : PB136714TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB136714TB

Quant Time: Jun 01 15:54:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration




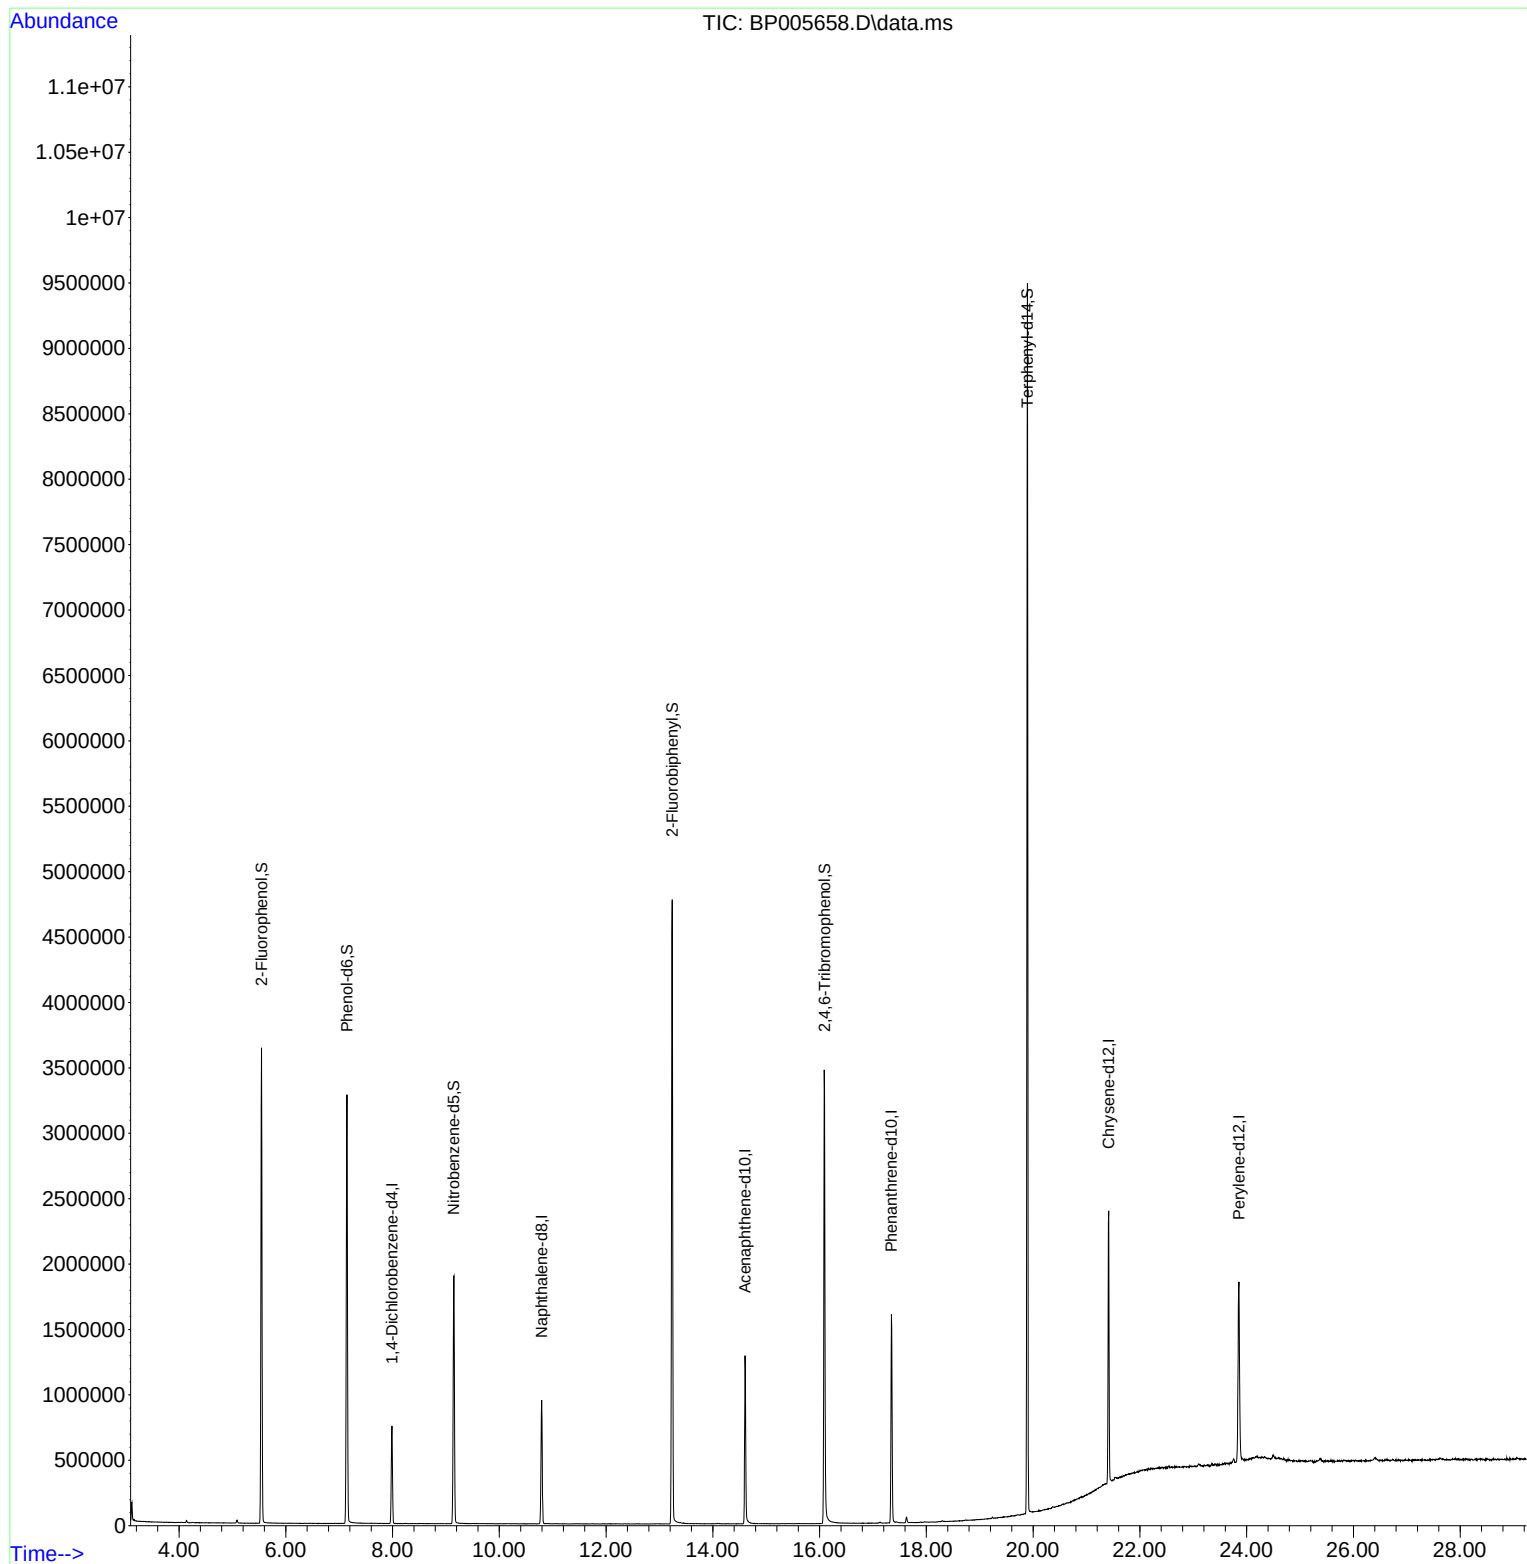


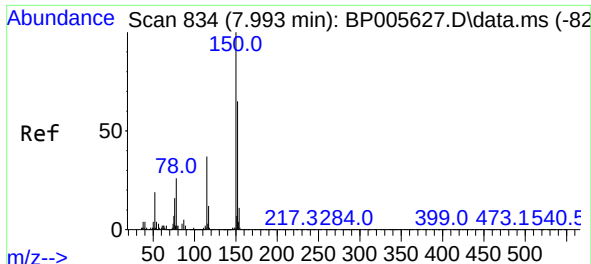

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.987 min Scan# 833
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17




Instrument :
BNA_P
ClientSampleId :
PB136714TB


Tgt Ion:152 Resp: 193597
Ion Ratio Lower Upper
152 100
150 156.5 119.8 179.8
115 57.8 49.0 73.4

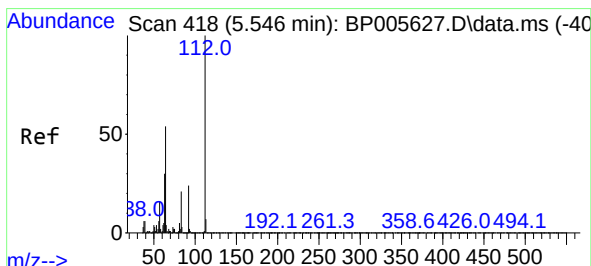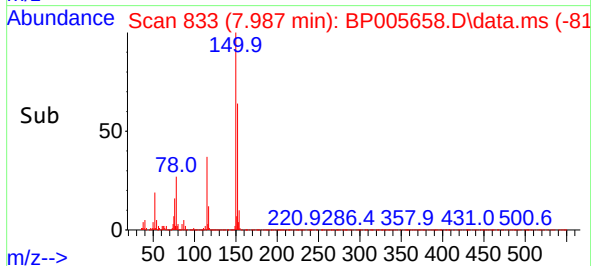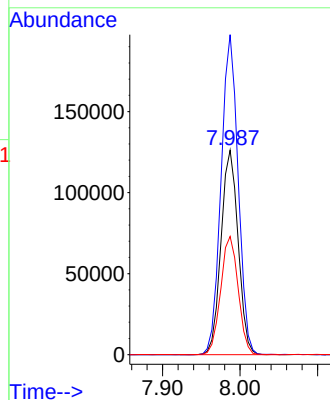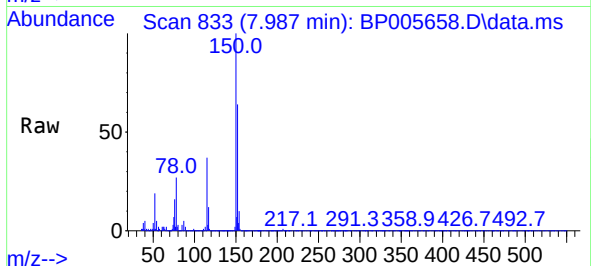

#5
2-Fluorophenol
Concen: 119.64 ng
RT: 5.546 min Scan# 418
Delta R.T. -0.000 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion:112 Resp: 1489820
Ion Ratio Lower Upper
112 100
64 54.8 33.6 50.4#
63 29.9 18.6 27.8#

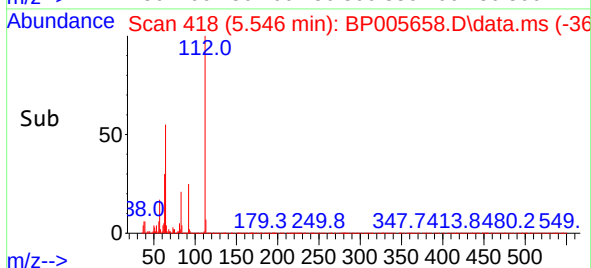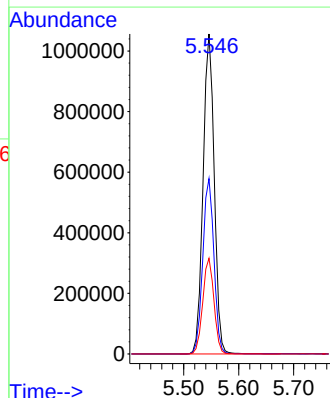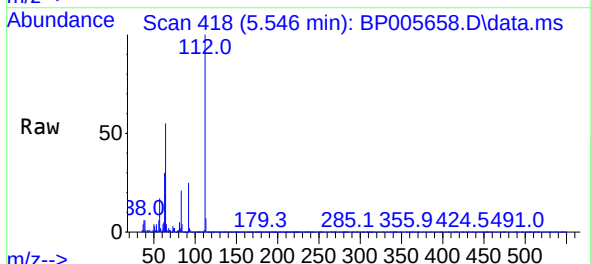




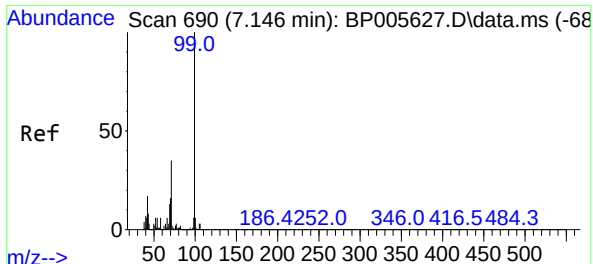


#7
Phenol-d6
Concen: 104.60 ng
RT: 7.146 min Scan# 690
Delta R.T. -0.000 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Instrument :
BNA_P
ClientSampleId :
PB136714TB

Tgt Ion: 99 Resp: 1775591




Ion	Ratio	Lower	Upper
99	100		
42	17.8	12.9	19.3
71	34.5	26.7	40.1

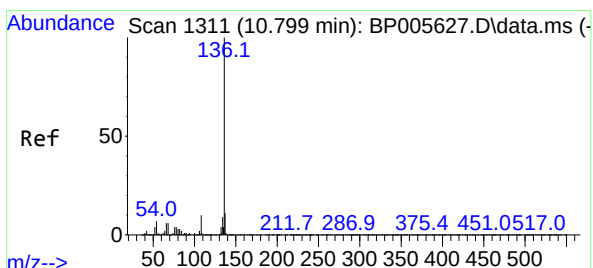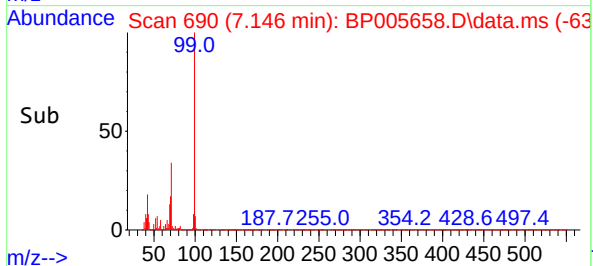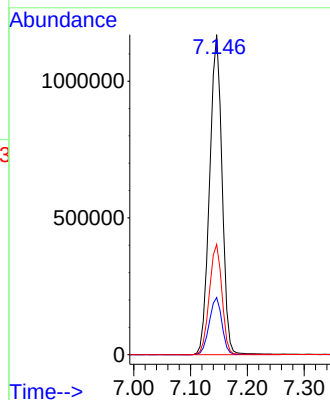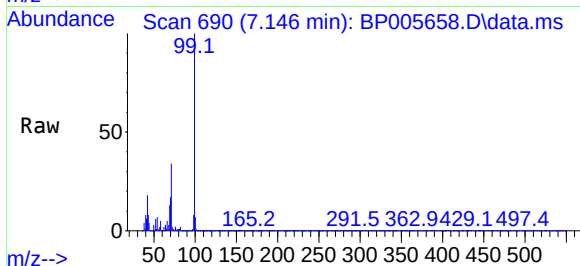


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.793 min Scan# 1310
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion:136 Resp: 759694

Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	6.9	5.0	7.4
68	5.6	3.7	5.5

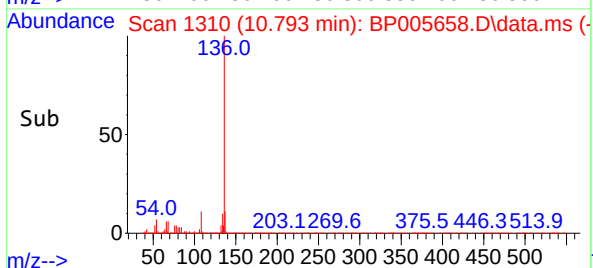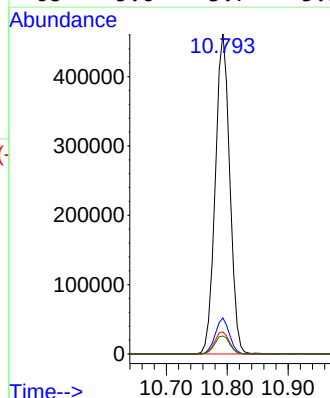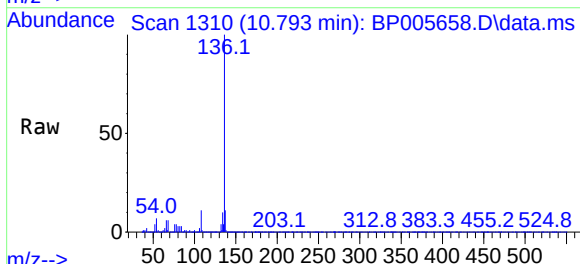




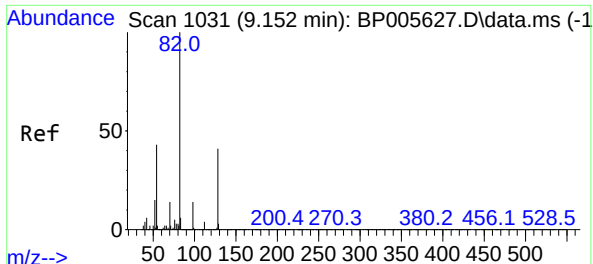


#23
Nitrobenzene-d5
Concen: 79.95 ng
RT: 9.146 min Scan# 1030
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Instrument :
BNA_P
ClientSampleId :
PB136714TB

Tgt Ion: 82 Resp: 1092158




Ion	Ratio	Lower	Upper
82	100		
128	40.9	30.5	45.7
54	43.5	33.9	50.9

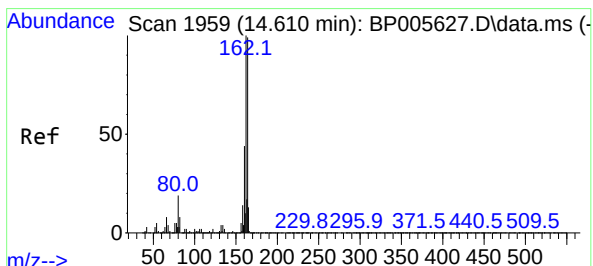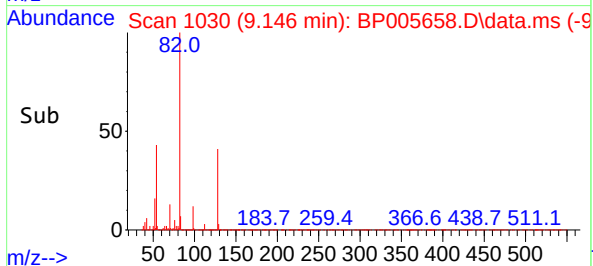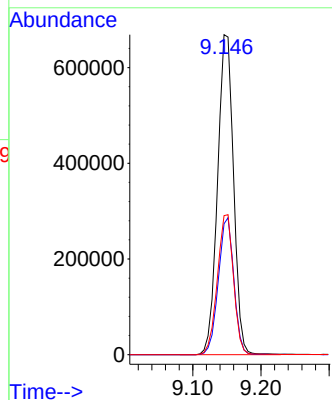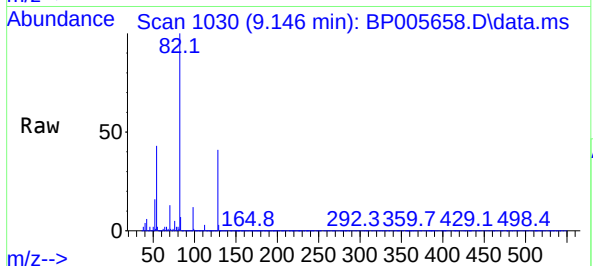


#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.604 min Scan# 1958
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion: 164 Resp: 449918

Ion	Ratio	Lower	Upper
164	100		
162	100.6	73.5	110.3
160	44.6	40.6	61.0


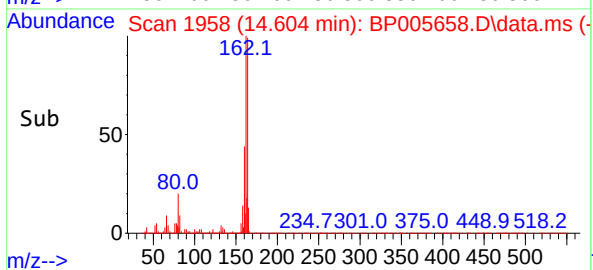
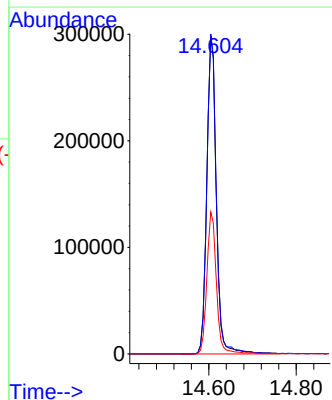
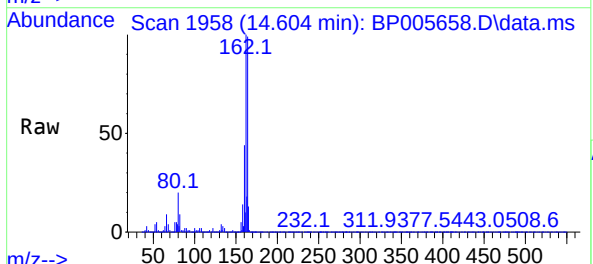


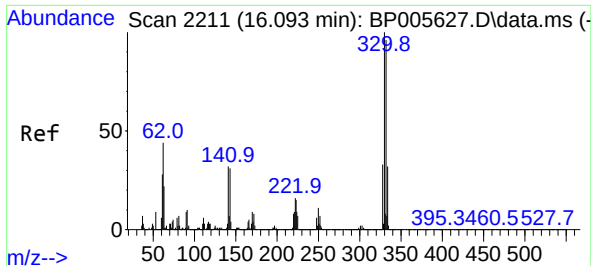

#42
2,4,6-Tribromophenol
Concen: 118.29 ng
RT: 16.092 min Scan# 2211
Delta R.T. -0.000 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17




Instrument :
BNA_P
ClientSampleId :
PB136714TB


Tgt Ion:330 Resp: 682422
Ion Ratio Lower Upper
330 100
332 96.3 76.3 114.5
141 31.6 22.8 34.2

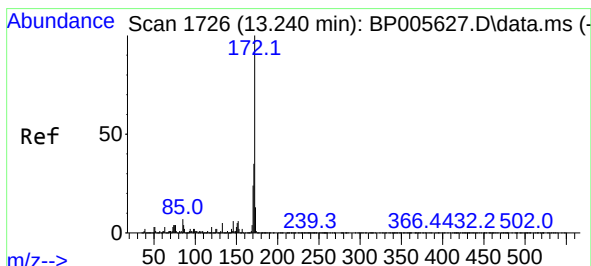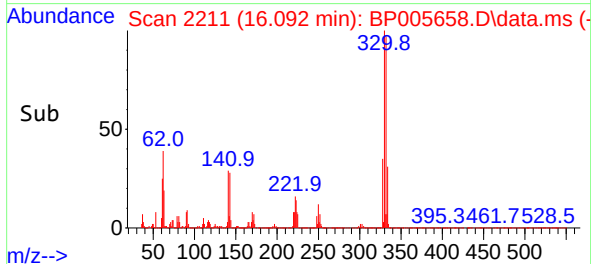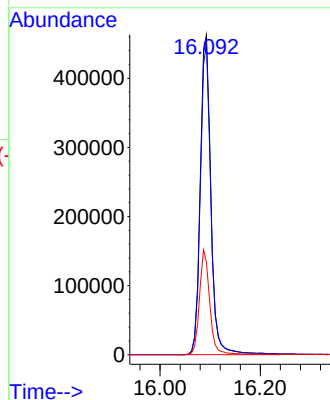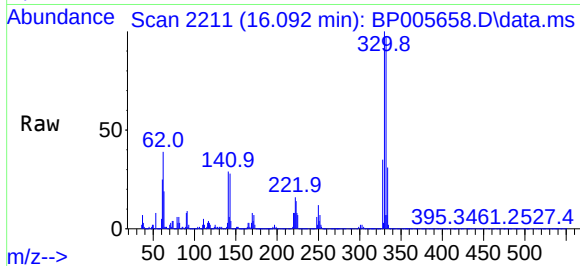

#45
2-Fluorobiphenyl
Concen: 71.82 ng
RT: 13.240 min Scan# 1726
Delta R.T. -0.000 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion:172 Resp: 2441536
Ion Ratio Lower Upper
172 100
171 34.9 28.1 42.1
170 23.6 19.6 29.4


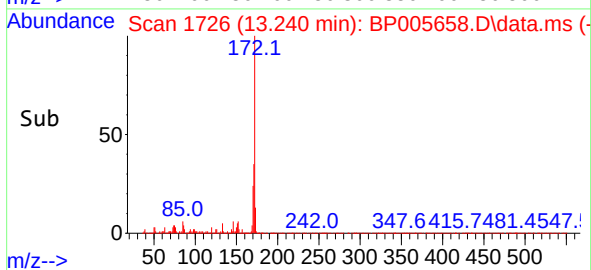
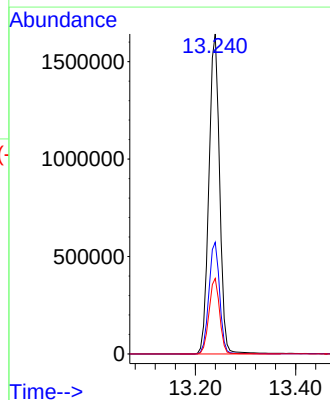
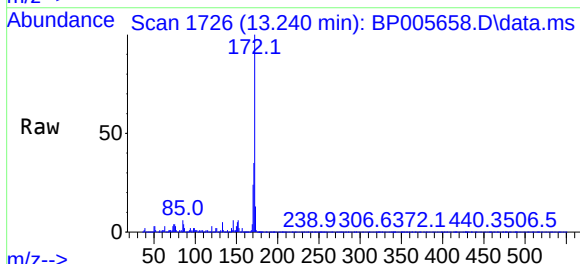


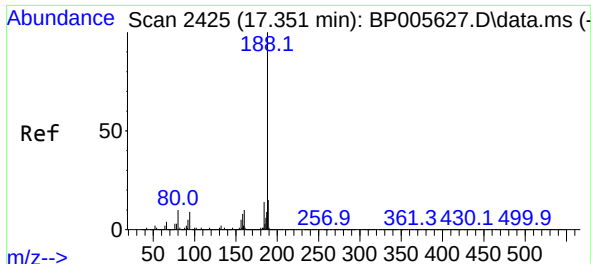

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.345 min Scan# 2424
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17




Instrument :
BNA_P
ClientSampleId :
PB136714TB


Tgt Ion:188 Resp: 959640
Ion Ratio Lower Upper
188 100
94 8.9 5.0 7.6#
80 9.6 5.9 8.9#

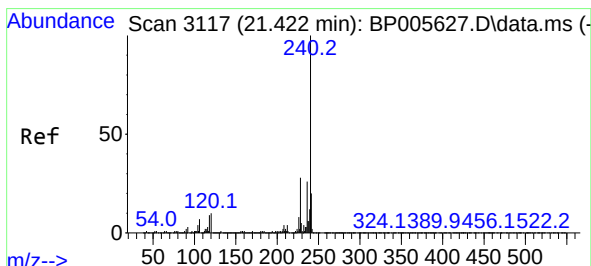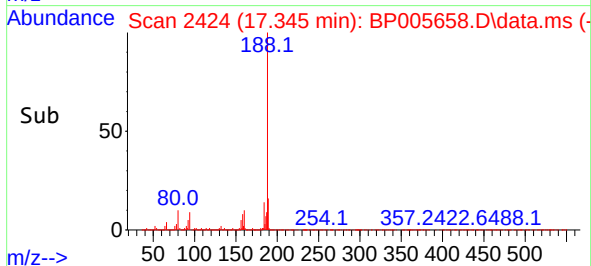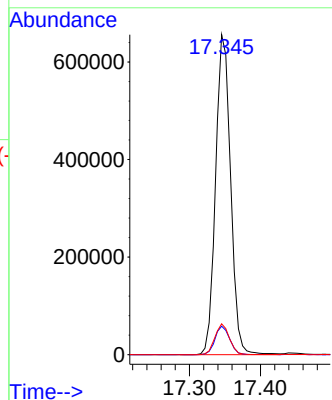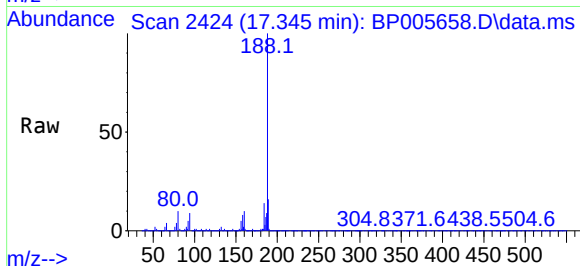

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.416 min Scan# 3116
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion:240 Resp: 982529
Ion Ratio Lower Upper
240 100
120 8.9 4.2 6.2#
236 25.5 20.2 30.2


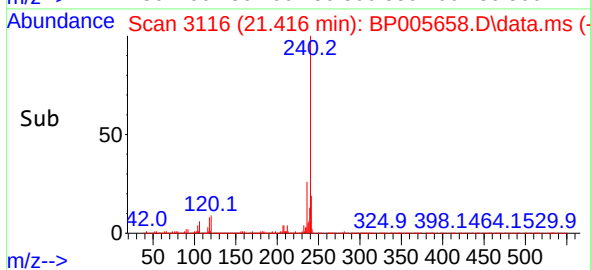
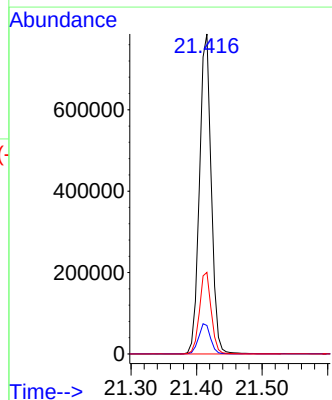
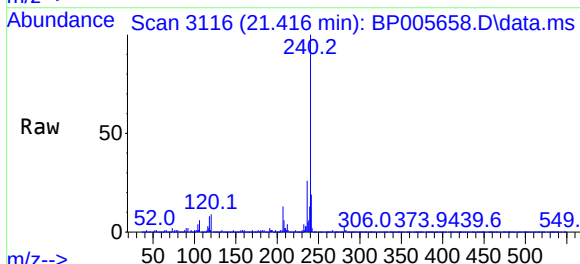


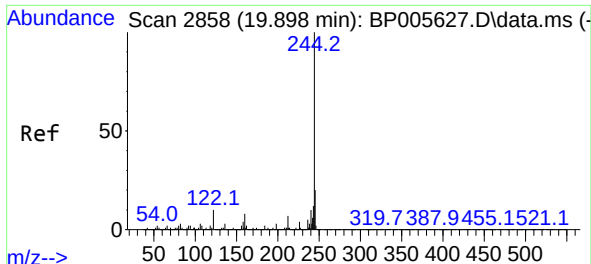

#79
Terphenyl-d14
Concen: 78.04 ng
RT: 19.892 min Scan# 2857
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Instrument :
BNA_P
ClientSampleId :
PB136714TB

Tgt Ion:244 Resp: 4086078
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.6
122 10.0 5.2 7.8#

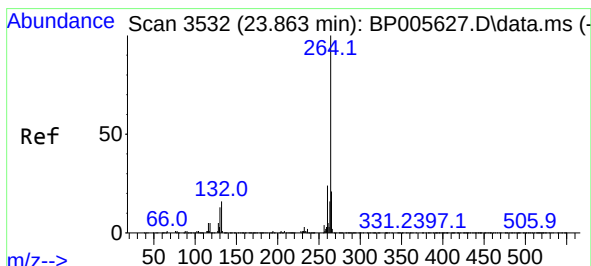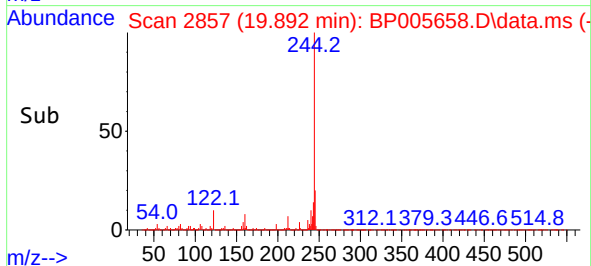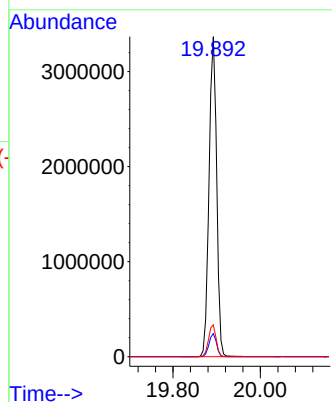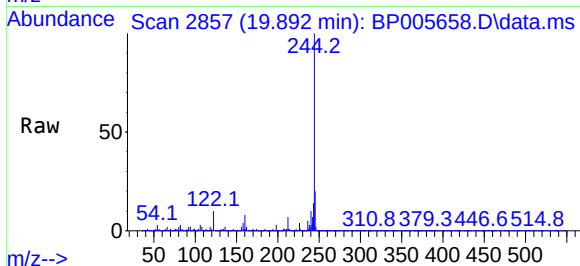

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.857 min Scan# 3531
Delta R.T. -0.006 min
Lab File: BP005658.D
Acq: 01 Jun 2021 15:17

Tgt Ion:264 Resp: 1027049
Ion Ratio Lower Upper
264 100
260 24.3 20.6 30.8
265 21.9 19.0 28.6

