
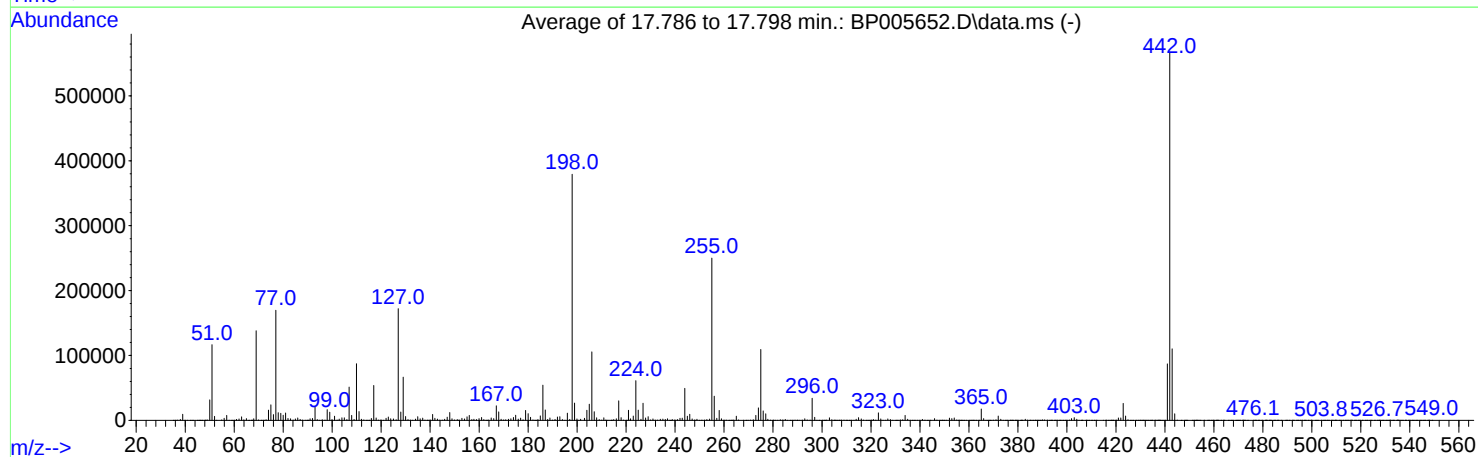


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\
 Data File : BP005652.D
 Acq On : 01 Jun 2021 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 16:11:11 2021

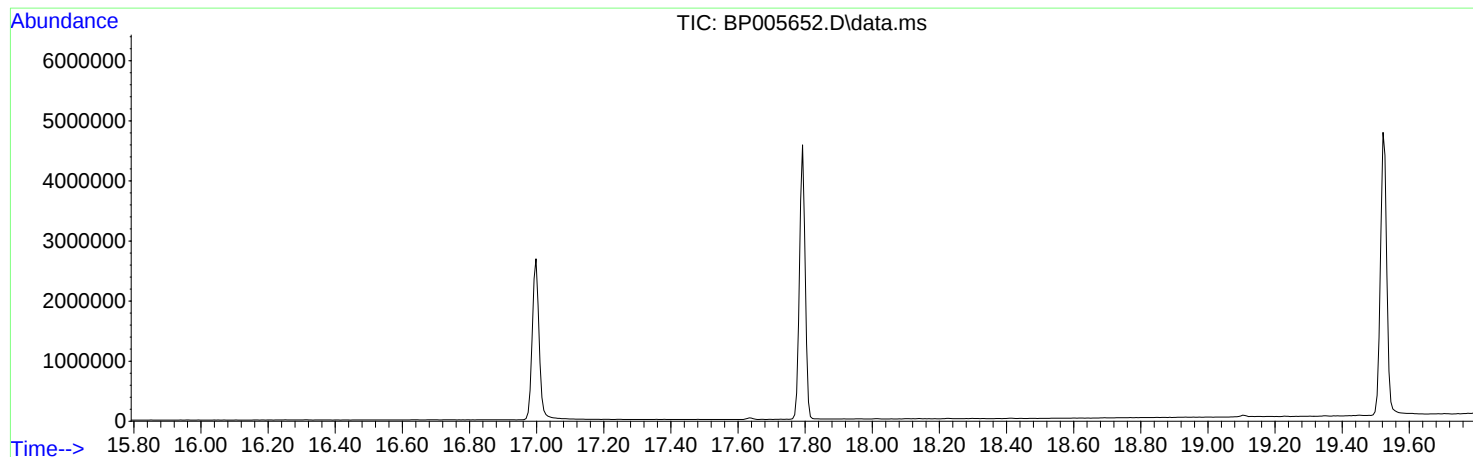




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	116672	PASS
68	69	0.00	2	1.7	2370	PASS
69	198	0.00	100	36.4	138047	PASS
70	69	0.00	2	0.5	694	PASS
127	198	10	80	45.3	172041	PASS
197	198	0.00	2	0.4	1573	PASS
198	198	100	100	100.0	379386	PASS
199	198	5	9	7.0	26655	PASS
275	198	10	60	28.8	109165	PASS
365	198	1	100	4.6	17620	PASS
441	198	0.01	100	22.9	86997	PASS
442	442	100	100	100.0	566927	PASS
443	442	15	24	19.4	110224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\
 Data File : BP005652.D
 Acq On : 01 Jun 2021 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jun 01 11:16:51 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 16:11:11 2021
 Response via : Initial Calibration

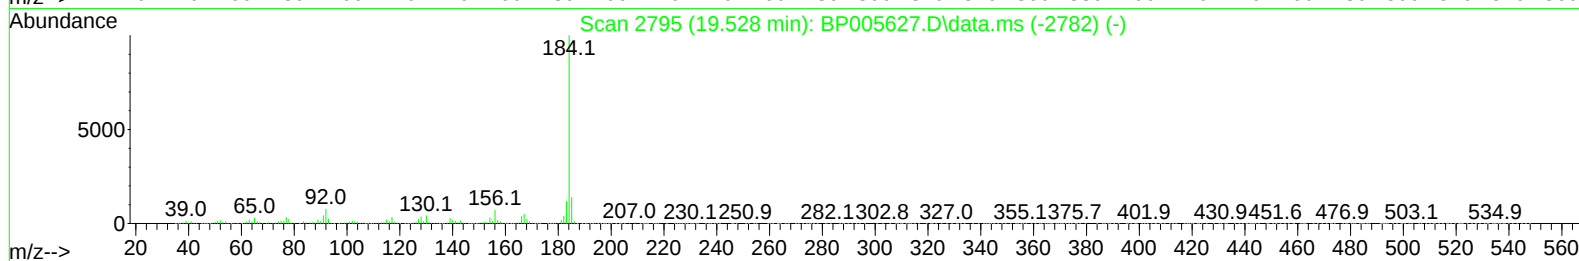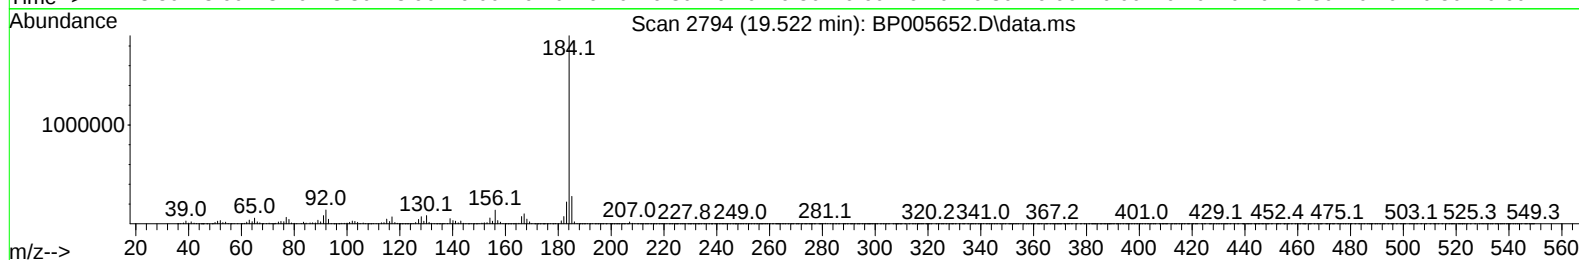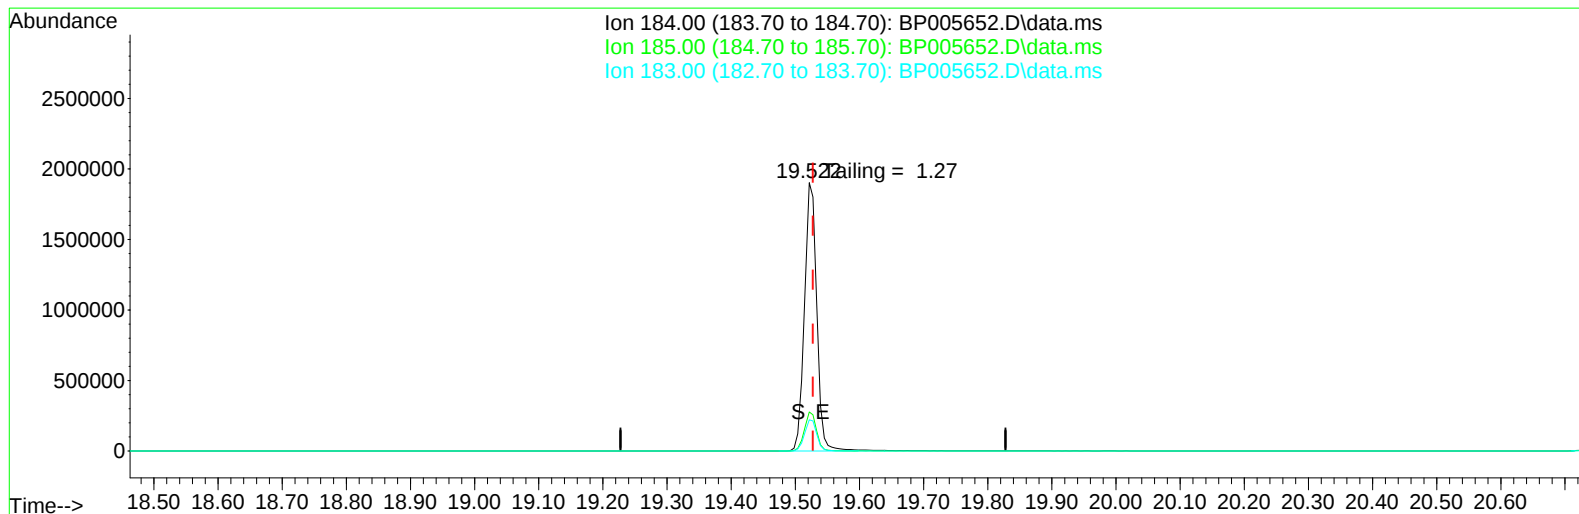

TIC: BP005652.D\data.ms

(77) Benzidine

19.522min (-0.006) 188155.35 ng




response 2551347

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.59
183.00	12.30	11.62
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP060121\  
Data File : BP005652.D  
Acq On    : 01 Jun 2021  10:30  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jun 01 11:16:51 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP052721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 16:11:11 2021
Response via : Initial Calibration

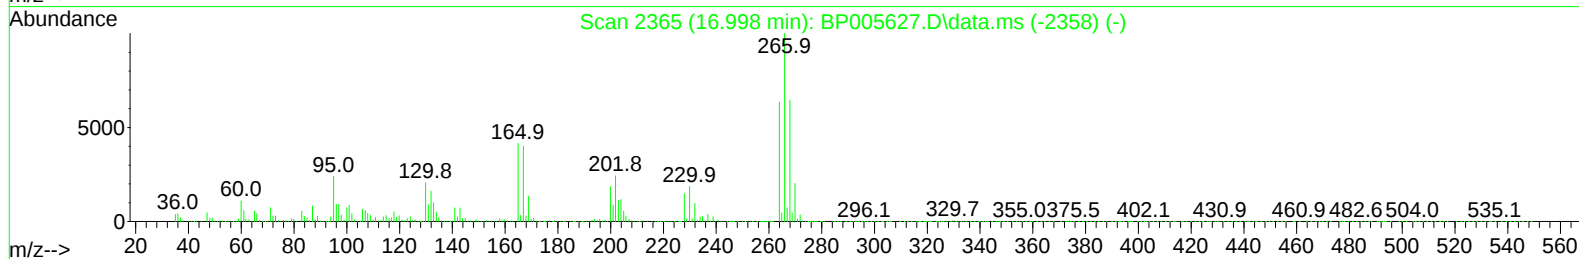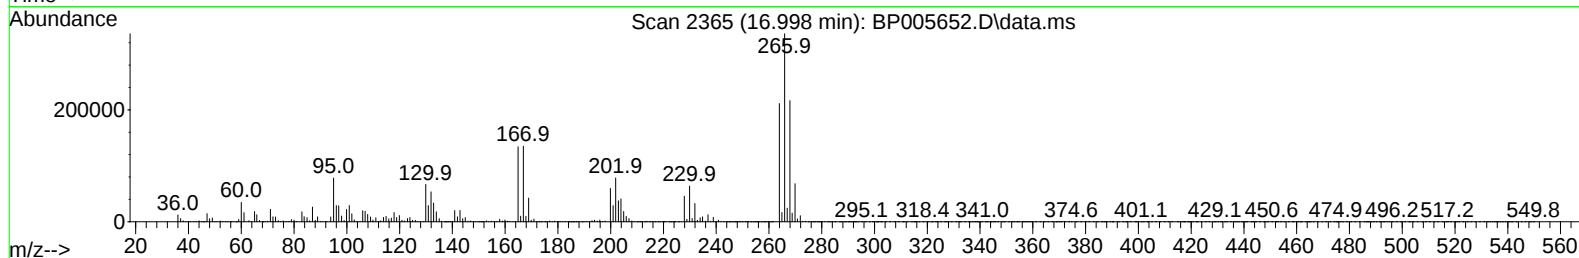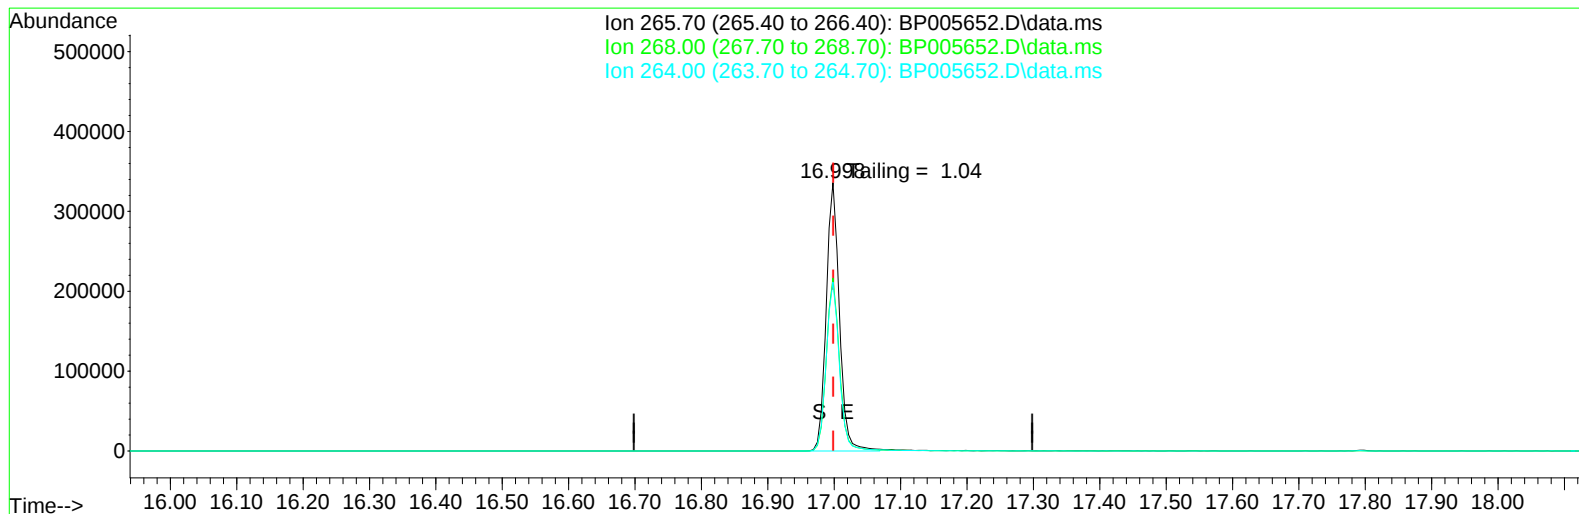

TIC: BP005652.D\data.ms

(70) Pentachlorophenol (C)

16.998min (-0.000) 182785.02 ng

response **466813**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.42
264.00	67.10	62.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/1/2021	BNA_P	<u>BP005652.D</u>
Compound Name	Response	Retention Time
DDT	1353092	20.72
DDD	7276	20.29
DDE	3102	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10378	1363470	0.76